



State of West Virginia
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Post Office Box 50130
 Charleston, WV 25305-0130

Request for Quotation

RFQ NUMBER
 WEH70232

PAGE
 1

ADDRESS/CONTACT INFORMATION/ATTENTION OF
 ROBERTA WAGNER
 304-558-0067

RFQ COPY
 TYPE NAME/ADDRESS HERE

VENDOR

Longs' Security Camera Systems LLC
 102 38th Street SE
 Charleston, WV 25304

SHIP TO

HEALTH AND HUMAN RESOURCES
 WELCH COMMUNITY HOSPITAL
 454 MCDOWELL STREET
 WELCH, WV 24801
 304-436-8710

DATE PRINTED	TERMS OF SALE	SHIP VIA	FOB	FREIGHT TERMS
05/23/2007				
BID OPENING DATE: 06/07/2007		BID OPENING TIME: 01:30PM		

LINE	QUANTITY	UOP	CAT NO.	ITEM NUMBER	UNIT PRICE	AMOUNT
0001	1	EA	725-40	NEW NURSE CALL SYSTEM (SEE ATTACHED SPECIFICATIONS)		\$143,000.00
ADDENDUM NO. 1 1. TO PROVIDE FLOOR PLANS, PER THE ATTACHED. 2. ADDENDUM ACKNOWLEDGEMENT IS ATTACHED. THIS DOCUMENT SHOULD BE SIGNED AND RETURNED WITH YOUR BID. FAILURE TO SIGN AND RETURN MAY RESULT IN DISQUALIFICATION OF YOUR BID. END OF ADDENDUM NO. 1 SEE ATTACHED SPEC SHEETS OF EQUIPMENT TO be provided						
***** THIS IS THE END OF RFQ WEH70232 ***** TOTAL:						

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE: *Alan C. King* TELEPHONE: 925-0038 DATE: 6-7-07

TITLE: Owner FEIN: 20-38881880 ADDRESS: CHANGES TO BE NOTED ABOVE

WHEN RESPONDING TO RFQ INSERT NAME AND ADDRESS IN SPACE ABOVE LABELLED 'VENDOR'

PURCHASING CONTINUATION SHEET

Report No.:	Req. or P.O. No.:
17-22	WEH70232
Funding:	

Vendor:

Requisition No.: 232

ADDENDUM ACKNOWLEDGEMENT

I hereby acknowledge receipt of the following addendum(s) and have made the necessary revisions to my proposal, plans and/or specifications, etc.

Addendum No.'s:

- No. 1
- No. 2
- No. 3
- No. 4
- No. 5

I understand that failure to confirm the receipt of the addendum(s) may be cause for rejection of bids.

Alan E. Long
 Signature
Long's Security Camera Sys LLC
 Company
06-07-07
 Date



State of West Virginia
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Post Office Box 50130
 Charleston, WV 25305-0130

Request for Quotation

RFQ NUMBER
WEH70232

PAGE
2

ADDRESS CORRESPONDENCE TO ATTENTION OF
**ROBERTA WAGNER
 304-558-0067**

RFQ COPY
 TYPE NAME/ADDRESS HERE

VENDOR

SHIP TO

**HEALTH AND HUMAN RESOURCES
 WELCH COMMUNITY HOSPITAL**

**454 MCDOWELL STREET
 WELCH, WV
 24801 304-436-8710**

DATE PRINTED	TERMS OF SALE	SHIP VIA	FOB	FREIGHT TERMS
05/07/2007				

BID OPENING DATE: **06/07/2007** BID OPENING TIME **01:30PM**

LINE	QUANTITY	UOP	CAT NO.	ITEM NUMBER	UNIT PRICE	AMOUNT
<p>BUSINESS ON MAY 22, 2007. QUESTIONS MAY BE SENT VIA USPS, FAX, COURIER, OR E-MAIL. IN ORDER TO ASSURE NO VENDOR RECEIVES AN UNFAIR ADVANTAGE, NO SUBSTANTIVE QUESTIONS WILL BE ANSWERED ORALLY. IF POSSIBLE, E-MAIL QUESTIONS ARE PREFERRED. ADDRESS INQUIRIES TO:</p> <p>ROBERTA WAGNER DEPARTMENT OF ADMINISTRATION PURCHASING DIVISION 2019 WASHINGTON STREET, EAST CHARLESTON, WV 25311</p> <p>FAX: 304-558-4115 E-MAIL: RWAGNER@WVADMIN.GOV</p> <p>THE MODEL/BRAND/SPECIFICATIONS NAMED HEREIN ESTABLISH THE ACCEPTABLE LEVEL OF QUALITY ONLY AND ARE NOT INTENDED TO REFLECT A PREFERENCE OR FAVOR ANY PARTICULAR BRAND OR VENDOR. VENDORS WHO ARE BIDDING ALTERNATES SHOULD SO STATE AND INCLUDE PERTINENT LITERATURE AND SPECIFICATIONS. FAILURE TO PROVIDE INFORMATION FOR ANY ALTERNATES MAY BE GROUNDS FOR REJECTION OF THE BID. THE STATE RESERVES THE RIGHT TO WAIVE MINOR IRREGULARITIES IN BIDS OR SPECIFICATIONS IN ACCORDANCE WITH SECTION 148-1-4(F) OF THE WEST VIRGINIA LEGISLATIVE RULES AND REGULATIONS.</p> <p>EXHIBIT 5</p> <p>NOTICE TO PROCEED: THIS CONTRACT IS TO BE PERFORMED WITHIN 120 CALENDAR DAYS AFTER THE NOTICE TO PROCEED IS RECEIVED. A "NOTICE TO PROCEED" LETTER WILL BE ISSUED INDICATING APPROVAL OF THE CONTRACTOR'S FINAL</p>						

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE <i>Alan E. King</i>	TELEPHONE 304-925-0338	DATE 06-07-07
TITLE <i>Owner</i>	FEIN 20-38881880	ADDRESS CHANGES TO BE NOTED ABOVE

WHEN RESPONDING TO RFQ. INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED 'VENDOR'



State of West Virginia
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Post Office Box 50130
 Charleston, WV 25305-0130

Request for Quotation

RFQ NUMBER
WEH70232

PAGE
3

ADDRESS CORRESPONDENCE TO ATTENTION OF
**ROBERTA WAGNER
 304-558-0067**

RFQ COPY
 TYPE NAME/ADDRESS HERE

HEALTH AND HUMAN RESOURCES
 WELCH COMMUNITY HOSPITAL

 454 MCDOWELL STREET
 WELCH, WV
 24801 304-436-8710

DATE PRINTED	TERMS OF SALE	SHIP VIA	F.O.B.	FREIGHT TERMS
05/07/2007				

BID OPENING DATE: **06/07/2007** BID OPENING TIME **01:30PM**

LINE	QUANTITY	UOP	CAT NO.	ITEM NUMBER	UNIT PRICE	AMOUNT
<p>DRAFT OF THE SHOP DRAWINGS.</p> <p>CANCELLATION: THE DIRECTOR OF PURCHASING RESERVES THE RIGHT TO CANCEL THIS CONTRACT IMMEDIATELY UPON WRITTEN NOTICE TO THE VENDOR IF THE MATERIALS OR WORKMANSHIP SUPPLIED ARE OF AN INFERIOR QUALITY OR DO NOT CONFORM WITH THE SPECIFICATIONS OF THE BID AND CONTRACT HERE IN.</p> <p>WAGE RATES: THE CONTRACTOR OR SUBCONTRACTOR SHALL PAY THE HIGHER OF THE U.S. DEPARTMENT OF LABOR MINIMUM WAGE RATES AS ESTABLISHED FOR MCDOWELL COUNTY, PURSUANT TO WEST VIRGINIA CODE 21-5A, ET, SEQ. (PREVAILING WAGE RATES APPLY TO THIS PROJECT)</p> <p>ARBITRATION: ANY REFERENCES MADE TO ARBITRATION OR INTEREST FOR PAYMENTS DUE (EXCEPT FOR ANY INTEREST REQUIRED BY STATE LAW) CONTAINED IN THIS CONTRACT OR IN ANY AMERICAN INSTITUTE OF ARCHITECTS DOCUMENTS PERTAINING TO THIS CONTRACT ARE HEREBY DELETED.</p> <p>WORKERS' COMPENSATION: VENDOR IS REQUIRED TO PROVIDE A CERTIFICATE FROM WORKERS' COMPENSATION IF SUCCESSFUL.</p> <p>ALL OF THE ITEMS CHECKED BELOW WILL BE A REQUIREMENT OF THIS CONTRACT:</p> <p>(XX) INSURANCE: SUCCESSFUL VENDOR SHALL FURNISH PROOF OF COMMERCIAL GENERAL LIABILITY INSURANCE PRIOR TO ISSUANCE OF CONTRACT. UNLESS OTHERWISE SPECIFIED IN THE BID DOCUMENTS, THE MINIMUM AMOUNT OF INSURANCE COVERAGE REQUIRED IS \$250,000.</p> <p>() BUILDERS RISK INSURANCE: SUCCESSFUL VENDOR SHALL FURNISH PROOF OF BUILDERS RISK - ALL RISK INSURANCE IN AN AMOUNT EQUAL TO 100% OF THE AMOUNT OF THE CONTRACT.</p>						

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE <i>Robert Wagner</i>	TELEPHONE 304-925-0338	DATE 06-07-07
TITLE OWNER	FEIN 20-38881880	ADDRESS CHANGES TO BE NOTED ABOVE

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED 'VENDOR'



State of West Virginia
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Post Office Box 50130
 Charleston, WV 25305-0130

Request for Quotation

RFQ NUMBER
WEH70232

PAGE
4

ADDRESS CORRESPONDENCE TO ATTENTION OF
**ROBERTA WAGNER
 304-558-0067**

RFQ COPY
 TYPE NAME/ADDRESS HERE

VENDOR

SHIP TO

**HEALTH AND HUMAN RESOURCES
 WELCH COMMUNITY HOSPITAL**

**454 MCDOWELL STREET
 WELCH, WV
 24801 304-436-8710**

DATE PRINTED	TERMS OF SALE	SHIP VIA	FOB	FREIGHT TERMS
05/07/2007				

BID OPENING DATE: **06/07/2007** BID OPENING TIME **01:30PM**

LINE	QUANTITY	UOP	CAT NO	ITEM NUMBER	UNIT PRICE	AMOUNT
<p>(XX) BONDS: FIVE PERCENT (5%) OF THE TOTAL AMOUNT OF THE BID PAYABLE TO THE STATE OF WEST VIRGINIA, SHALL BE SUBMITTED WITH EACH BID AS A BID BOND. THE SUCCESSFUL BIDDER SHALL ALSO FURNISH A PERFORMANCE BOND AND LABOR/MATERIAL BOND FOR 100% OF THE AMOUNT OF THE CONTRACT. BONDS MAY BE PROVIDED IN THE FORM OF A CERTIFIED CHECK, IRREVOCABLE LETTER OF CREDIT, OR BOND FURNISHED BY A SOLVENT SURETY COMPANY AUTHORIZED TO DO BUSINESS IN THE STATE OF WEST VIRGINIA. A LETTER OF CREDIT SUBMITTED IN LIEU OF A PERFORMANCE AND LABOR & MATERIAL BOND WILL ONLY BE ALLOWED FOR PROJECTS UNDER \$100,000. PERSONAL OR BUSINESS CHECKS ARE NOT ACCEPTABLE IN LIEU OF THE 5% BID BOND, PERFORMANCE BOND, OR LABOR AND MATERIAL BOND.</p> <p>() MAINTENANCE BOND: A TWO (2) YEAR MAINTENANCE BOND COVERING THE ROOFING SYSTEM WILL BE A REQUIREMENT OF THE SUCCESSFUL VENDOR.</p> <p>REV. 11/00</p> <p>EXHIBIT 7</p> <p>DOMESTIC ALUMINUM, GLASS & STEEL IN PUBLIC WORKS PROJECTS</p> <p>IN ACCORDANCE WITH WEST VIRGINIA CODE 5-19-1 ET., SEQ., EVERY CONTRACT FOR CONSTRUCTION, RECONSTRUCTION, ALTERATION, REPAIR, IMPROVEMENT OR MAINTENANCE OF PUBLIC WORKS, WHERE THE COST IS MORE THAN \$50,000 AND, IN THE CASE OF STEEL ONLY, WHERE THE COST OF STEEL IS MORE THAN \$50,000 OR WHERE MORE THAN 10,000 POUNDS OF STEEL ARE REQUIRED, THE STATE WILL ACCEPT ONLY ALUMINUM GLASS, OR STEEL PRODUCTS PRODUCED IN THE UNITED STATES</p>						

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE <i>Edman E. King</i>	TELEPHONE 304-925-0338	DATE 06-07-07
TITLE <i>Owner</i>	ADDRESS CHANGES TO BE NOTED ABOVE	

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED 'VENDOR'



State of West Virginia
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Post Office Box 50130
 Charleston, WV 25305-0130

Request for Quotation

RFQ NUMBER:
WEH70232

PAGE:
5

ADDRESS CORRESPONDENCE TO ATTENTION OF:
**ROBERTA WAGNER
 304-558-0067**

RFQ COPY
 TYPE NAME/ADDRESS HERE

VENDOR

SHIP TO

**HEALTH AND HUMAN RESOURCES
 WELCH COMMUNITY HOSPITAL**

**454 MCDOWELL STREET
 WELCH, WV
 24801 304-436-8710**

DATE PRINTED	TERMS OF SALE	SHIP VIA	F.O.B.	FREIGHT TERMS
05/07/2007				

BID OPENING DATE: **06/07/2007** BID OPENING TIME **01:30PM**

LINE	QUANTITY	UOP	CAT NO	ITEM NUMBER	UNIT PRICE	AMOUNT
<p>IN ADDITION, ITEMS OF MACHINERY OR EQUIPMENT PURCHASED FOR USE AT THE SITE OF PUBLIC WORKS SHALL BE MADE OF DOMESTIC ALUMINUM, GLASS OR STEEL, UNLESS THE COST OF THE PRODUCT IS LESS THAN \$50,000 OR LESS THAN 10,000 POUNDS OF STEEL ARE USED IN PUBLIC WORKS PROJECTS.</p> <p>FOREIGN MADE ALUMINUM, GLASS OR STEEL PRODUCTS MAY BE ACCEPTED ONLY IF THE COST OF DOMESTIC PRODUCTS IS FOUND TO BE UNREASONABLE. SUCH COST IS UNREASONABLE IF IT IS 20% OR MORE HIGHER THAN THE BID PRICE FOR FOREIGN MADE PRODUCTS. IF THE DOMESTIC ALUMINUM, GLASS OR STEEL PRODUCTS TO BE SUPPLIED OR PRODUCED IN A "SUBSTANTIAL LABOR SURPLUS AREA", AS DEFINED BY THE UNITED STATES DEPARTMENT OF LABOR, FOREIGN PRODUCTS MAY BE SUPPLIED ONLY IF DOMESTIC PRODUCTS ARE 30% OR MORE HIGHER IN PRICE THAN THE FOREIGN MADE PRODUCTS.</p> <p>IF, PRIOR TO THE AWARD OF A CONTRACT UNDER THE ABOVE PROVISIONS, THE SPENDING OFFICER OF THE SPENDING UNIT DETERMINES THAT THERE EXISTS A BID FOR LIKE FOREIGN ALUMINUM, GLASS OR STEEL THAT IS REASONABLE AND LOWER THAN THE LOWEST BID DOMESTIC PRODUCTS, THE SPENDING OFFICE MAY REQUEST, IN WRITING, A REEVALUATION AND REDUCTION IN THE LOWEST BID FOR SUCH DOMESTIC PRODUCTS ALL VENDORS MUST INDICATE IN THEIR BID IF THEY ARE SUPPLYING FOREIGN ALUMINUM, GLASS OR STEEL.</p> <p>REV. 3/88</p> <p>EXHIBIT 9</p> <p>NOTICE FOR ISSUANCE & ACKNOWLEDGEMENT OF CONSTRUCTION PROJECT ADDENDA</p> <p>THE ARCHITECT/ENGINEER AND/OR AGENCY SHALL BE REQUIRED</p>						

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE <i>William E. Long</i>	TELEPHONE 304-925-0338	DATE 06-07-07
TITLE <i>Owner</i>	FEIN 20-38881880	ADDRESS CHANGES TO BE NOTED ABOVE

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED 'VENDOR'



State of West Virginia
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Post Office Box 50130
 Charleston, WV 25305-0130

Request for Quotation

RFQ NUMBER:
WEH70232

PAGE:
6

ADDRESS CORRESPONDENCE TO ATTENTION OF:
**ROBERTA WAGNER
 304-558-0067**

RFQ COPY
 TYPE NAME/ADDRESS HERE

VENDOR

SHIP TO

**HEALTH AND HUMAN RESOURCES
 WELCH COMMUNITY HOSPITAL**

**454 MCDOWELL STREET
 WELCH, WV
 24801 304-436-8710**

DATE PRINTED	TERMS OF SALE	SHIP VIA	F.O.B.	FREIGHT TERMS
05/07/2007				

BID OPENING DATE: **06/07/2007** BID OPENING TIME **01:30PM**

LINE	QUANTITY	UOP	CAT NO.	ITEM NUMBER	UNIT PRICE	AMOUNT
<p>TO ABIDE BY THE FOLLOWING SCHEDULE IN ISSUING CONSTRUCTION PROJECT ADDENDA FOR STATE AGENCIES:</p> <p>(1) THE ARCHITECT/ENGINEER SHALL PREPARE THE ADDENDUM AND A LIST OF ALL PARTIES THAT HAVE PROCURED DRAWINGS AND SPECIFICATIONS FOR THE PROJECT. THE ADDENDUM AND LIST SHALL BE FORWARDED TO THE BUYER IN THE STATE PURCHASING DIVISION. THE ARCHITECT/ENGINEER SHALL ALSO SEND A COPY OF THE ADDENDUM TO THE STATE AGENCY FOR WHICH THE CONTRACT IS ISSUED.</p> <p>(2) THE BUYER SHALL SEND THE ADDENDUM TO ALL INTERESTED PARTIES AND, IF NECESSARY, EXTEND THE BID OPENING DATE. ANY ADDENDUM SHOULD BE RECEIVED BY THE BUYER WITHIN FOURTEEN (14) DAYS PRIOR TO THE BID OPENING DATE.</p> <p>(3) ALL ADDENDA SHOULD BE FORMALLY ACKNOWLEDGED BY ALL BIDDERS AND SUBMITTED TO THE STATE PURCHASING DIVISION. THE SAME RULES AND REGULATIONS THAT APPLY TO THE ORIGINAL BIDDING DOCUMENT SHALL ALSO APPLY TO AN ADDENDUM DOCUMENT. THE ONLY EXCEPTION MAY BE FOR AN ADDENDUM THAT IS ISSUED FOR THE SOLE PURPOSE OF CHANGING A BID OPENING TIME AND/OR DATE.</p> <p>REV. 11/96</p> <p>EXHIBIT 10</p> <p>ADDENDUM ACKNOWLEDGEMENT</p> <p>I HEREBY ACKNOWLEDGE RECEIPT OF THE FOLLOWING CHECKED ADDENDUM(S) AND HAVE MADE THE NECESSARY REVISIONS TO MY PROPOSAL, PLANS AND/OR SPECIFICATION, ETC.</p>						

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE <i>Alan E. King</i>	TELEPHONE 304-925-0338	DATE 06-07-07
TITLE <i>Owner</i>	FEIN 20-39881980	ADDRESS CHANGES TO BE NOTED ABOVE

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED 'VENDOR'



State of West Virginia
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Post Office Box 50130
 Charleston, WV 25305-0130

Request for Quotation

RFQ NUMBER:
WEH70232

PAGE:
7

ADDRESS CORRESPONDENCE TO ATTENTION OF:
**ROBERTA WAGNER
 304-558-0067**

RFQ COPY
 TYPE NAME/ADDRESS HERE

VENDOR

SHIP TO

**HEALTH AND HUMAN RESOURCES
 WELCH COMMUNITY HOSPITAL**

**454 MCDOWELL STREET
 WELCH, WV
 24801 304-436-8710**

DATE PRINTED	TERMS OF SALE	SHIP VIA	FOB	FREIGHT TERMS
05/07/2007				

BID OPENING DATE: **06/07/2007** BID OPENING TIME **01:30PM**

LINE	QUANTITY	UOP	CAT NO	ITEM NUMBER	UNIT PRICE	AMOUNT
ADDENDUM NOS.:						
NO. 1
NO. 2
NO. 3
NO. 4
NO. 5
I UNDERSTAND THAT FAILURE TO CONFIRM THE RECEIPT OF THE ADDENDUM(S) MAY BE CAUSE FOR REJECTION OF THE BIDS.						
<i>Alan E. King</i>				SIGNATURE		
<i>Long Security Camera Systems LLC</i>				COMPANY		
<i>06-07-07</i>				DATE		
REV. 11/96						
CONTRACTORS LICENSE						
WEST VIRGINIA STATE CODE 21-11-2 REQUIRES THAT ALL PERSONS DESIRING TO PERFORM CONTRACTING WORK IN THIS STATE MUST BE LICENSED. THE WEST VIRGINIA CONTRACTORS LICENSING BOARD IS EMPOWERED TO ISSUE THE CONTRACTORS LICENSE. APPLICATIONS FOR A CONTRACTORS LICENSE MAY BE MADE BY CONTACTING THE WEST VIRGINIA DIVISION OF LABOR CAPITOL COMPLEX, BUILDING 3, ROOM 319, CHARLESTON, WV 25305. TELEPHONE: (304) 558-7890.						

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE <i>Alan E. King</i>	TELEPHONE <i>304-95-0338</i>	DATE <i>06-07-07</i>
TITLE <i>Owner</i>	FEIN <i>20-38881880</i>	ADDRESS CHANGES TO BE NOTED ABOVE

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED 'VENDOR'



State of West Virginia
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Post Office Box 50130
 Charleston, WV 25305-0130

Request for Quotation

RFQ NUMBER:
WEH70232

PAGE:
8

ADDRESS CORRESPONDENCE TO ATTENTION OF:
**ROBERTA WAGNER
 304-558-0067**

RFQ COPY
 TYPE NAME/ADDRESS HERE

VENDOR

SHIP TO

**HEALTH AND HUMAN RESOURCES
 WELCH COMMUNITY HOSPITAL**

**454 MCDOWELL STREET
 WELCH, WV
 24801 304-436-8710**

DATE PRINTED	TERMS OF SALE	SHIP VIA	FOB	FREIGHT TERMS
05/07/2007				

BID OPENING DATE: **06/07/2007** BID OPENING TIME **01:30PM**

LINE	QUANTITY	UOP	CAT NO	ITEM NUMBER	UNIT PRICE	AMOUNT
<p>WEST VIRGINIA STATE CODE 21-11-11 REQUIRES ANY PROSPECTIVE BIDDER TO INCLUDE THE CONTRACTORS LICENSE NUMBER ON THEIR BID.</p> <p>BIDDER TO COMPLETE:</p> <p>CONTRACTORS NAME: <i>Long Security Camera Systems LLC</i></p> <p>CONTRACTORS LICENSE NO.: <i>WV 040102</i></p> <p>THE SUCCESSFUL BIDDER WILL BE REQUIRED TO FURNISH A COPY OF THEIR CONTRACTORS LICENSE PRIOR TO ISSUANCE OF A PURCHASE ORDER/CONTRACT</p> <p>APPLICABLE LAW</p> <p>THE WEST VIRGINIA STATE CODE, PURCHASING DIVISION RULE AND REGULATIONS, AND THE INFORMATION PROVIDED IN THE "REQUEST FOR QUOTATION" ISSUED BY THE PURCHASING DIVISION IS THE SOLE AUTHORITY GOVERNING THIS PROCUREMENT.</p> <p>ANY INFORMATION PROVIDED IN SPECIFICATION MANUALS, OR ANY OTHER SOURCE, VERBAL OR WRITTEN, WHICH CONTRADICTS OR ALTERS THE INFORMATION PROVIDED FROM THE SOURCES AS DESCRIBED IN THE ABOVE PARAGRAPH IS VOID AND OF NO EFFECT.</p> <p>BANKRUPTCY: IN THE EVENT THE VENDOR/CONTRACTOR FILES FOR BANKRUPTCY PROTECTION, THIS CONTRACT IS AUTOMATICALLY NULL AND VOID, AND IS TERMINATED WITHOUT FURTHER ORDER.</p> <p>REV. 1/2005</p>						

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE <i>Alan E. King</i>	TELEPHONE <i>304-925-0338</i>	DATE <i>06-07-07</i>
TITLE <i>Owner</i>	FEIN <i>20-38881880</i>	ADDRESS CHANGES TO BE NOTED ABOVE

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED 'VENDOR'

STATE OF WEST VIRGINIA
Purchasing Division**PURCHASING AFFIDAVIT**

West Virginia Code §5A-3-10a states: No contract or renewal of any contract may be awarded by the state or any of its political subdivisions to any vendor or prospective vendor when the vendor or prospective vendor or a related party to the vendor or prospective vendor is a debtor and the debt owned is an amount greater than one thousand dollars in the aggregate

DEFINITIONS:

"Debt" means any assessment, premium, penalty, fine, tax or other amount of money owed to the state or any of its political subdivisions because of a judgment, fine, permit violation, license assessment, defaulted workers' compensation premium, penalty or other assessment presently delinquent or due and required to be paid to the state or any of its political subdivisions, including any interest or additional penalties accrued thereon.

"Debtor" means any individual, corporation, partnership, association, limited liability company or any other form or business association owing a debt to the state or any of its political subdivisions. "Political subdivision" means any county commission; municipality; county board of education; any instrumentality established by a county or municipality; any separate corporation or instrumentality established by one or more counties or municipalities, as permitted by law; or any public body charged by law with the performance of a government function or whose jurisdiction is coextensive with one or more counties or municipalities. "Related party" means a party, whether an individual, corporation, partnership, association, limited liability company or any other form or business association or other entity whatsoever, related to any vendor by blood, marriage, ownership or contract through which the party has a relationship of ownership or other interest with the vendor so that the party will actually or by effect receive or control a portion of the benefit, profit or other consideration from performance of a vendor contract with the party receiving an amount that meets or exceeds five percent of the total contract amount.

EXCEPTION: The prohibition of this section does not apply where a vendor has contested any tax administered pursuant to chapter eleven of this code, workers' compensation premium, permit fee or environmental fee or assessment and the matter has not become final or where the vendor has entered into a payment plan or agreement and the vendor is not in default of any of the provisions of such plan or agreement.

LICENSING: Vendors must be licensed and in good standing in accordance with any and all state and local laws and requirements by any state or local agency of West Virginia, including, but not limited to, the West Virginia Secretary of State's Office, the West Virginia Tax Department, West Virginia Insurance Commission, or any other state agencies or political subdivision. Furthermore, the vendor must provide all necessary releases to obtain information to enable the Director or spending unit to verify that the vendor is licensed and in good standing with the above entities.

CONFIDENTIALITY: The vendor agrees that he or she will not disclose to anyone, directly or indirectly, any such personally identifiable information or other confidential information gained from the agency, unless the individual who is the subject of the information consents to the disclosure in writing or the disclosure is made pursuant to the agency's policies, procedures and rules. Vendors should visit www.state.wv.us/admin/purchase/privacy for the Notice of Agency Confidentiality Policies.

Under penalty of law for false swearing (West Virginia Code, §61-5-3), it is hereby certified that the vendor acknowledges the information in this said affidavit and are in compliance with the requirements as stated.

Vendor's Name:

Longs Security Camera Systems LLC

Authorized Signature:

Alan E. Jung

Date:

06-07-07

AGREEMENT ADDENDUM

031

In the event of conflict between this addendum and the agreement, this addendum shall control:

1. **ARBITRATION** - Any references to arbitration contained in the agreement are hereby deleted. Disputes arising out of the agreement shall be presented to the West Virginia Court of Claims.
2. **HOLD HARMLESS** - Any clause requiring the Agency to indemnify or hold harmless any party is hereby deleted in its entirety.
3. **GOVERNING LAW** - The agreement shall be governed by the laws of the State of West Virginia. This provision replaces any references to any other State's governing law.
4. **TAXES** - Provisions in the agreement requiring the Agency to pay taxes are deleted. As a State entity, the Agency is exempt from Federal, State, and local taxes and will not pay taxes for any Vendor including individuals, nor will the Agency file any tax returns or reports on behalf of Vendor or any other party.
5. **PAYMENT** - Any references to prepayment are deleted. Payment will be in arrears.
6. **INTEREST** - Should the agreement include a provision for interest on late payments, the Agency agrees to pay the maximum legal rate under West Virginia law. All other references to interest or late charges are deleted.
7. **RECOUPMENT** - Any language in the agreement waiving the Agency's right to set-off, counterclaim, recoupment, or other defense is hereby deleted.
8. **FISCAL YEAR FUNDING** - Service performed under the agreement may be continued in succeeding fiscal years for the term of the agreement, contingent upon funds being appropriated by the Legislature or otherwise being available for this service. In the event funds are not appropriated or otherwise available for this service, the agreement shall terminate without penalty on June 30. After that date, the agreement becomes of no effect and is null and void. However, the Agency agrees to use its best efforts to have the amounts contemplated under the agreement included in its budget. Non-appropriation or non-funding shall not be considered an event of default.
9. **STATUTE OF LIMITATION** - Any clauses limiting the time in which the Agency may bring suit against the Vendor, lessor, individual, or any other party are deleted.
10. **SIMILAR SERVICES** - Any provisions limiting the Agency's right to obtain similar services or equipment in the event of default or non-funding during the term of the agreement are hereby deleted.
11. **ATTORNEY FEES** - The Agency recognizes an obligation to pay attorney's fees or costs only when assessed by a court of competent jurisdiction. Any other provision is invalid and considered null and void.
12. **ASSIGNMENT** - Notwithstanding any clause to the contrary, the Agency reserves the right to assign the agreement to another State of West Virginia agency, board or commission upon thirty (30) days written notice to the Vendor and Vendor shall obtain the written consent of Agency prior to assigning the agreement.
13. **LIMITATION OF LIABILITY** - The Agency, as a State entity, cannot agree to assume the potential liability of a Vendor. Accordingly, any provision limiting the Vendor's liability for direct damages or limiting the Vendor's liability under a warranty to a certain dollar amount or to the amount of the agreement is hereby deleted. In addition, any limitation is null and void to the extent that it precludes any action for injury to persons or for damages to personal property.
14. **RIGHT TO TERMINATE** - Agency shall have the right to terminate the agreement upon thirty (30) days written notice to Vendor.
15. **TERMINATION CHARGES** - Any provision requiring the Agency to pay a fixed amount or liquidated damages upon termination of the agreement is hereby deleted. The Agency may only agree to reimburse a Vendor for actual costs incurred or losses sustained during the current fiscal year due to wrongful termination by the Agency prior to the end of any current agreement term.
16. **RENEWAL** - Any reference to automatic renewal is hereby deleted. The agreement may be renewed only upon mutual written agreement of the parties.
17. **INSURANCE** - Any provision requiring the Agency to insure equipment or property of any kind and name the Vendor as beneficiary or as an additional insured is hereby deleted.
18. **RIGHT TO NOTICE** - Any provision for repossession of equipment without notice is hereby deleted. However, the Agency does recognize a right of repossession with notice.
19. **ACCELERATION** - Any reference to acceleration of payments in the event of default or non-funding is hereby deleted.
20. **AMENDMENTS** - All amendments, modifications, alterations or changes to the agreement shall be in writing and signed by both parties. No amendment, modification, alteration or change may be made to this addendum without the express written approval of the Purchasing Division and the Attorney General.

ACCEPTED BY:
STATE OF WEST VIRGINIA

Spending Unit: _____

Signed: _____

Title: _____

Date: _____

VENDOR

Company Name: Long's Security America Systems LLC

Signed: Alan C. Long

Title: Owner

Date: 06-07-07

CONTRACTOR LICENSE

Authorized by the

West Virginia Contractor Licensing Board

Number: WV040102

Classification:

LOW VOLTAGE SYSTEMS

LONGS SECURITY CAMERA SYSTEMS LLC
102 38TH STREET SE
CHARLESTON, WV 25304

Date Issued

Expiration Date

JANUARY 26, 2007

JANUARY 26, 2008

Authorized Company Signature

Michael A. Carl

Chair, West Virginia Contractor
Licensing Board

WEST VIRGINIA
CONTRACTOR
LICENSING
BOARD

This license, or a copy thereof, must be posted in a conspicuous place at every construction site where work is being performed. This license number must appear in all advertisements, on all bid submissions and on all fully executed and binding contracts. This license cannot be assigned or transferred by licensee. Issued under provisions of West Virginia Code, Chapter 21, Article 11.

JUN/07/2007/THU 09:20 AM

2.00


ACORD CERTIFICATE OF LIABILITY INSURANCE		DATE(MM/DD/YYYY) 06/07/2007
PRODUCER Insurance Intermediaries, Inc. 6460 Busch Blvd., Suite 100 Columbus, OH 43229-1717		THIS CERTIFICATE IS ISSUED AS A MATTER OF INFORMATION ONLY AND CONFERS NO RIGHTS UPON THE CERTIFICATE HOLDER. THIS CERTIFICATE DOES NOT AMEND, EXTEND OR ALTER THE COVERAGE AFFORDED BY THE POLICIES BELOW.
INSURED Long's Security Camera Systems LLC 102 38th St SE Charleston, WV 25304		
INSURERS AFFORDING COVERAGE		NAIC#
INSURER A: Scottsdale Insurance Co.		
INSURER B:		
INSURER C:		
INSURER D:		
INSURER E:		

COVERAGES

THE POLICIES OF INSURANCE LISTED BELOW HAVE BEEN ISSUED TO THE INSURED NAMED ABOVE FOR THE POLICY PERIOD INDICATED. NOTWITHSTANDING ANY REQUIREMENT, TERM OR CONDITION OF ANY CONTRACT OR OTHER DOCUMENT WITH RESPECT TO WHICH THIS CERTIFICATE MAY BE ISSUED OR MAY PERTAIN, THE INSURANCE AFFORDED BY THE POLICIES DESCRIBED HEREIN IS SUBJECT TO ALL THE TERMS, EXCLUSIONS AND CONDITIONS OF SUCH POLICIES. AGGREGATE LIMITS SHOWN MAY HAVE BEEN REDUCED BY PAID CLAIMS.

INSTR. NO. / TR. INSTR.	TYPE OF INSURANCE	POLICY NUMBER	POLICY EFFECTIVE DATE(MM/DD/YYYY)	POLICY EXPIRATION DATE(MM/DD/YYYY)	LIMITS
A	GENERAL LIABILITY <input checked="" type="checkbox"/> COMMERCIAL GENERAL LIABILITY <input type="checkbox"/> CLAIMSMADE <input checked="" type="checkbox"/> OCCUR GEN'L AGGREGATE LIMIT APPLIES PER: <input type="checkbox"/> POLICY <input type="checkbox"/> OCC. <input type="checkbox"/> TRGT. <input type="checkbox"/> LOC	CL51367547	02/19/2007	02/19/2008	EACH OCCURRENCE \$ 200,000 DAMAGE TO RENTED PREMISES (EA OCCURRENCE) \$ 100,000 MED EXP (Any one person) \$ 5,000 PERSONAL & ADV. INJURY \$ 200,000 GENERAL AGGREGATE \$ 600,000 PRODUCTS - COMP/OP AGG \$ 600,000
	AUTOMOBILE LIABILITY <input type="checkbox"/> ANY AUTO <input type="checkbox"/> ALL OWNED AUTOS <input type="checkbox"/> SCHEDULED AUTOS <input type="checkbox"/> HIRED AUTOS <input type="checkbox"/> NON-OWNED AUTOS				COMBINED SINGLE LIMIT (EA ACCIDENT) \$ BODILY INJURY (Per person) \$ BODILY INJURY (Per accident) \$ PROPERTY DAMAGE (Per accident) \$ AUTO ONLY - EA ACCIDENT \$ OTHER THAN AUTO ONLY: EA ACC \$ ADD \$ EACH OCCURRENCE \$ AGGREGATE \$ \$ \$ \$ WC STATUTORY LIMITS BOTH \$ E.L. EACH ACCIDENT \$ E.L. DISEASE - EA EMPLOYEE \$ E.L. DISEASE - POLICY LIMIT \$
	GARAGE LIABILITY <input type="checkbox"/> ANY AUTO				
	EXCESS/UMBRELLA LIABILITY <input type="checkbox"/> OCCUR <input type="checkbox"/> CLAIMSMADE <input type="checkbox"/> DEDUCTIBLE RETENTION \$				
	WORKERS COMPENSATION AND EMPLOYERS' LIABILITY ANY PROPRIETOR/PARTNER/EXECUTIVE OFFICER/OWNER EXCLUDED? If yes, describe under SPECIAL PROVISIONS below OTHER				

DESCRIPTION OF OPERATIONS / LOCATIONS / VEHICLES / EXCLUSIONS ADDED BY ENDORSEMENT / SPECIAL PROVISIONS

CERTIFICATE HOLDER Health & Human Resources Welch Community Hospital 453 McDowell St Welch, WV 24806	CANCELLATION SHOULD ANY OF THE ABOVE DESCRIBED POLICIES BE CANCELLED BEFORE THE EXPIRATION DATE THEREOF, THE ISSUING INSURER WILL ENDEAVOR TO MAIL 30 DAYS WRITTEN NOTICE TO THE CERTIFICATE HOLDER NAMED TO THE LEFT, BUT FAILURE TO DO SO SHALL IMPOSE NO OBLIGATION OR LIABILITY OF ANY KIND UPON THE INSURER, ITS AGENTS OR REPRESENTATIVES. AUTHORIZED REPRESENTATIVE 
---	---

Agency Purchasing
REQ. P. O. # WEH70232
Bond # 13437

BID BOND

KNOW ALL MEN BY THESE PRESENTS, That we, the undersigned, Long's Security Camera System, LLC.
of 102 38th St. S.E., Charleston, WV 25304, as Principal, and American Southern Insurance
Company of 7512 Slate Ridge Blvd. Reynoldsburg, OH 43068, a corporation organized and existing under the laws of the State of Kansas
with its principal office in the City of Atlanta, GA, as Surety, are held and firmly bound unto the State
of West Virginia, as Obligee, in the penal sum of Eight Thousand Five Hundred Twenty Five and No/100 (\$8,525.00) for the payment of which,
well and truly to be made, we jointly and severally bind ourselves, our heirs, administrators, executors, successors and assigns.

The Condition of the above obligation is such that whereas the Principal has submitted to the Purchasing Section of the
Department of Administration a certain bid or proposal, attached hereto and made a part hereof, to enter into a contract in writing for
Nurse Call System at Welch Hospital, WEH 70232

NOW THEREFORE,

- (a) If said bid shall be rejected, or
- (b) If said bid shall be accepted and the Principal shall enter into a contract in accordance with the bid or proposal attached hereto and shall furnish any other bonds and insurance required by the bid or proposal, and shall in all other respects perform the agreement created by the acceptance of said bid, then this obligation shall be null and void, otherwise this obligation shall remain in full force and effect. It is expressly understood and agreed that the liability of the Surety for any and all claims hereunder shall, in no event, exceed the penal amount of this obligation as herein stated.

The Surety, for the value received, hereby stipulates and agrees that the obligations of said Surety and its bond shall be in no way impaired or affected by any extension of the time within which the Obligee may accept such bid, and said Surety does hereby waive notice of any such extension.

IN WITNESS WHEREOF, Principal and Surety have hereunto set their hands and seals, and such of them as are corporations have caused their corporate seals to be affixed hereunto and these presents to be signed by their proper officers, this
7th day of June, 2007.

Principal Corporate Seal

Long's Security Camera System, LLC.
(Name of Principal)
By [Signature]
(Must be President or Vice President)
Owner
(Title)

Surety Corporate Seal

American Southern Insurance Company
(Name of Surety)
[Signature]
Attorney-in-Fact
Andrew C. Heaner

IMPORTANT – Surety executing bonds must be licensed in West Virginia to transact surety insurance. Raised corporate seals must be affixed, a power of attorney must be attached.

AMERICAN SOUTHERN INSURANCE COMPANY

Home Office: 200 S.W. 30th Street
Topeka, Kansas 66611

Mailing Address: 3715 Northside Pkwy, NW
Bldg 400, Ste 800
Atlanta, Georgia 30327

GENERAL POWER OF ATTORNEY

Know all men by these Presents, that the American Southern Insurance Company had made, constituted and appointed, and by these presents does make, constitute and appoint Stefan E. Tauger of Parker, Colorado; Arthur S. Johnson of Atlanta, Georgia; Jessica B. Gardiner of Loganville, Georgia; Mary F. Holland of Chamblee, Georgia; Donald H. Gibbs of Atlanta, Georgia; Andrew C. Heaner of Atlanta, Georgia; Richard L. Shanahan of Atlanta, Georgia; Katherine S. Grimsley of Tampa, Florida; Jeffery L. Booth of Parma, Ohio; James E. Feldner of West Lake Ohio; Cheryl L. Torrao of Canton, Georgia; Garry W. Black of Murfreesboro, Tennessee; Martha G. Ross of Charlotte, North Carolina; or David R. Brett of Columbia, South Carolina, EACH as its true and lawful attorney for it and its name, place and stead to execute on behalf of the said company, as surety, bonds, undertakings and contracts of suretyship to be given to all obligees provided that no bond or undertaking or contract of suretyship executed under this authority shall exceed in amount of the sum of \$850,000 (eight hundred fifty thousand dollars), including but not limited to consents of surety for the release of retained percentages and/or final estimates on construction contracts or similar authority requested by the Department of Transportation, State of Florida; and the execution of such undertakings, bonds, recognizances and other surety obligations, in pursuance of the presents, shall be as binding upon the Company as if they had been duly signed by the President and attested by the Secretary of the Company in their own proper persons.


This Power of Attorney is granted and is signed and sealed by facsimile under and by the authority of the following Resolution adopted pursuant to due authorization by the Executive Committee of the Board of Directors of the American Southern Insurance Company on the 26th day of May, 1998:

RESOLVED, that the Chairman, President or any Vice President of the Company be, and that each or any of them hereby is, authorized to execute Powers of Attorney qualifying the attorney named in the given Power of Attorney to execute in behalf of the American Southern Insurance Company bonds, undertakings and all contracts of suretyship; and that any Secretary or any Assistant Secretary be, and that each or any of them hereby is, authorized to attest the execution of any such Power of Attorney, and to attach thereto the seal of the Company.

FURTHER RESOLVED, that the signature of such officers and the seal of the Company may be affixed to any such Power of Attorney or to any certificate relating thereto by facsimile, and any such Power of Attorney or certificate bearing such facsimile signatures or facsimile seal shall be valid and binding upon the Company when so affixed and in the future, with respect to any bond undertaking or contract of suretyship to which it is attached.


In Witness Whereof, the American Southern Insurance Company has caused its official seal to be hereto affixed, and these presents to be signed by its President and attested by its Secretary this 7th day of December, 2006.

Attest:


Gail A. Lee, Secretary

By:

American Southern Insurance Company


Scott G. Thompson, President

STATE OF GEORGIA

SS:

COUNTY OF FULTON

On this 7th day of December, 2006, before me personally came Scott G. Thompson to me known, who being by me duly sworn, did depose and say that he resides in Atlanta, in the County of Fulton, State of Georgia, at 421 Hollydale Court; that he is the President of American Southern Insurance Company, the corporation described in and which executed the above instrument; that he knows the seal of the said corporation; that the seal affixed to the said instrument is such corporate seal; that it was so affixed and that he signed his name thereto pursuant to the authorization.

STATE OF GEORGIA

SS:

COUNTY OF FULTON


Melonie A. Coppola
Notary Public, State of Georgia
Qualified in Cobb County


Commission Expires May 17, 2010

I, the undersigned, a Vice President of American Southern Insurance Company, a Kansas Corporation, DO HEREBY CERTIFY that the foregoing and attached Power of Attorney remains in full force and has not been revoked; and, furthermore, that the Resolution of the Executive Committee of the Board of Directors set forth in the Power of Attorney is now in force.

Signed and sealed at the City of Atlanta, Dated the 7th day of June, 2007.

Number 13437

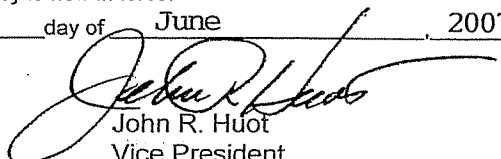
John R. Huot
Vice President

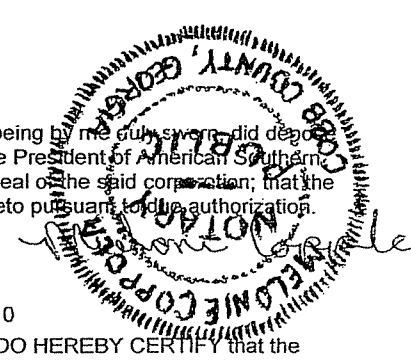

State of West Virginia
Offices of the Insurance Commissioner
Certificate of Authority


Whereas, AMERICAN SOUTHERN INSURANCE COMPANY domiciled in the State of Kansas has complied with all the requirements of the laws of this State so as to entitle it to transact its appropriate business in the State of West Virginia.

Therefore, I the undersigned, Insurance Commissioner of the State of West Virginia, pursuant to the authority vested in me by the laws of this State, do hereby authorize it to transact the business of insurance as defined in Chapter 33

ARTICLE 1, SECTION 10(c) -- FIRE
ARTICLE 1, SECTION 10(d) -- MARINE
ARTICLE 1, SECTION 10(e) -- CASUALTY
ARTICLE 1, SECTION 10(f) (1) (2) & (3) -- SURETY

of the 1931 Code of West Virginia as amended, in the State of West Virginia in accordance with the laws thereof until midnight on the 31st day of May, 2007, unless this license be sooner revoked. Pursuant to W. Va. Code 33-3-2(c), the above authorization does not allow the insurer to transact a kind of insurance in this State unless duly authorized or qualified to transact such insurance in the state or country of its domicile.

In Testimony Whereof, I have hereunto set my hand and affixed my seal of office at the City of Charleston this 1st day of June, 2006.


Jane L. Cline
Insurance Commissioner



WV File #0063

American Southern Insurance Company
 NAIC Company Code 10235
 NAIC Group Code 587

Statutory Financial Statement


As of December 31, 2006

ASSETS		LIABILITIES	
Bonds	\$54,206,267	Reserve for Losses and Loss Expense	\$33,388,259
Stocks	26,239,019	Reserve for Unearned Premiums	21,217,908
Cash and Short-Term Investments	11,444,228	Reserve for Expenses, Taxes, Licenses and Fees	9,057,867
Agents Balances or Uncollected with Reinsured Companies	9,466,223	Payable to Parents, Subsidiaries and Affiliates	273,203
Other Assets	3,170,263	Other Liabilities	5,650,917
		Total Liabilities	69,588,154
		POLICYHOLDERS' SURPLUS	
		Capital Stock	3,000,000
		Surplus	31,937,846
		Total Policyholders' Surplus	34,937,846
Total Assets	\$104,526,000	Total Liabilities and Policyholders' Surplus	\$104,526,000


Bonds and stocks are valued in accordance with the basis adopted by the National Association of Insurance Commissioners (NAIC).

CERTIFICATE

The officers of this reporting entity being duly sworn, each depose and say that they are the described officers of said reporting entity, and that on the reporting period stated above, all of the herein described assets were the absolute property of the said reporting entity, free and clear from any liens or claims thereon, except as herein stated, and that this statement, together with related exhibits, schedules and explanations therein contained, annexed or referred to, is a full and true statement of all the assets and liabilities and of the condition and affairs of the said reporting entity as of the reporting period stated above, and of its income and deductions therefrom for the period ended, and have been completed in accordance with the NAIC Annual Statement Instructions and Accounting Practices and Procedures manual except to the extent that: (1) state law may differ; or, (2) that state rules or regulations require differences in reporting not related to accounting practices and procedures, according to the best of their information, knowledge and belief, respectively.




 President



 Treasurer/Controller

State of Georgia
 County of Fulton

On the 26th day of January 2007, before me came the above named officers of the American Southern Insurance Company to me personally known to be the individuals and officers described herein, and acknowledge that they executed the foregoing instrument and affixed the seal of said company thereto by authority of their office.



 Melonie Coppola, Notary Public
 My Commission Expires, May 17, 2010



Tek-CARE®NC300II NC304 and NC304LCD Master Station Specification Sheet

IL693
Section E
Rev. 5-11/2006



NC304 Master Station



NC304LCD Master Station

ARCHITECTS' AND ENGINEERS' SPECIFICATION

The nurses' master station shall be TekTone® NC304, NC304LCD or approved equal. The master station wiring shall be supervised. The master station shall include the necessary signaling circuitry and firmware to receive and answer calls from all patient, staff, and duty stations; and receive calls from code and emergency stations on the Tek-CARE®NC300II System.

The master station shall provide for handset or loudspeaker communication with patients and staff. Function buttons (with and without LEDs) shall be provided to initiate reset operation, staff emergency request, nurse/aide request, paging operations, and nurse-follower operations. Additional buttons for menu-driven programmable functions include: talk, monitor, capture and room priority programming.

For the NC304LCD, incoming calls shall be displayed by room numbers in plain English on an integral LCD display with a minimum of 2 lines capable of displaying 40 characters each. The calls will display in order of time of origination and in accordance with established priority. The master stations shall also provide a color VGA output to connect to a standard UL® 1069 Listed VGA monitor (TekTone®'s NC315) for color VGA call display. A parallel port and serial port shall be available for connection to UL® 1069 Listed devices.

The user shall be able to access system programming via the keys on the master station or via the keyboard port which will accept any standard PC keyboard.

The master station shall be equipped with an integral handset, volume control, color-keyed function buttons, tone-off button, call LED, busy LED, CE fault LED, 2.5" speaker, electrostatic microphone. The master station will also include a 12-button digital keypad for entry of station numbers, zone and station assignments, and for selection of menu functions. All buttons shall also switch to alpha-character operation by depressing the switch marked ALPHA. Alpha-character operation shall allow for alphanumeric room numbering, room labeling, and calling of rooms so designated. All switches shall be of spill-resistant membrane switch design.

Each master station shall be able to address up to 512 single or dual stations per system, and up to 16 individual zones. The Tek-CARE®NC300II System shall support up to 8 master stations. The master station shall be UL® 1069 listed.

The station housing shall be high-impact, flame-retardant (UL® 94V-0) plastic and shall be desk mounted.

www.tektone.NET

277 Industrial Park Road • Franklin, NC 28734 • Phone (828) 524-9967 • Fax (828) 524-9968
Email: tektone@tektone.net • Technical Assistance Email: teksupt@tektone.net
TekTone®'s quality system is registered by UL® to the ISO 9001:2000 standard. (File #A10766.)

FEATURES

A major component of the Tek-CARE®NC300II System, the NC304LCD and NC304 master station supplies the user interface to respond to calls, issue staff requests and alter room programming status to accommodate differing patient needs. The NC304LCD and NC304 are functionally the same but the NC304LCD has an integral 2 line, 80-character LCD display for showing up to 4 active calls.

The master console allows for room and staff communication by either open speaker or handset for additional privacy. A VGA monitor can be used (required for the NC304) to display up to 22 active patient, staff or duty calls as well as columns for two levels of staff presence and STAT priority calls in English language format.

Master function buttons are provided to select the system functions as follows:

RESET	(black)	Terminates most operations.
AIDE	(yellow)	Enters an aide service request.
NURSE	(green)	Enters a nurse service request.
STAT	(red)	Enters an urgent staff emergency request.
MENU	(blue)	Displays functions menu for programming additional features.
PAGE FOLLOW	(gray)	Initiates paging operations.
TALK	(orange)	Initiates nurse-follower operations.
	(white)	Press to speak, press again to listen when using loudspeaker for communications.
ALPHA	(white)	Changes all function keys to the specifically labeled alpha characters.
MONITOR	(blue)	Enables room monitoring.
CAPTURE	(blue)	Allows for zone assignment.
VIEW	(blue)	Allows review of station information.
PRIORITY	(blue)	Activates menu for changing room priority.
TONE ON	(white)	Turns normal call-tone on/off.

Additional programmable functions include set station priority, set privacy, zone assignments, view station configurations, set password, reset time of day, time display, set overtime, transfer for master stations, paging, system configuration, and system reinitialization.

The master station is also equipped with volume control for adjustment of incoming voice communication; tone switch for controlling the lowest priority tone signal only; call light with indication of low, medium and high priority calls; CE fault LED; busy and alphanumeric keypad used for entry of station numbers, zone and station selection, and for selection of menu functions.

The master stations also provide a parallel port and serial port for connection to UL® 1069 Listed devices. The system programming is accessible to the user via the keys on the master station or via the keyboard port which will accept any standard PC keyboard.

- UL® 1069 Listed
- Supervised
- VGA output, Parallel port, Serial & Keyboard ports
- Spill-proof membrane switch with alphabetic characters
- Easy access to commonly used menu functions
- Simultaneous display of 22 calls
- Electrostatic microphone for clear voice communications
- Simple, menu-driven programmable functions
- Master-to-master intercom capability
- Single-button or handset intercom
- Calls displayed by priority and origination
- Calls identified by room and bed number
- Programmable patient priority and privacy
- Calls-waiting, calls-overtime and cord-out indication
- View station configuration capability
- Initiate STAT staff emergency request
- Upgrade patient call
- Distinct tones for high, medium and low-priority calls
- Nurse follower function
- Paging by zone or to all staff
- Overhead paging interface
- Patient monitor single or group
- Manual tone-silencing switch (for Routine calls only)
- High priority calls override tone-off feature
- Simplified multiplex wiring uses plug-in type connectors
- Continuous display of nurse/aide location and nurse/aide requested
- Use masters in parallel or independently

SPECIFICATIONS

Dimensions:	Console: 10.75" × 8.75" × 3.25"
Capacity:	Address up to 512 single or dual patient stations in up to 16 zones
Environments:	26°C, relative humidity should not exceed 80%
Terminations:	Plug-on connectors
System protection:	All outputs are protected by self-resetting current-limiting devices


REQUIRED COMPONENTS

NC315	Flat Panel VGA Monitor
NC351(A)	Central Equipment (4 masters/256 stations)
-or-	
NC351(A)/2	Central Equipment (8 masters/512 stations)
IR300C series	Patient Stations



NC351A and NC351A/2 Central Equipment Specification Sheet

IL696
Section E
Rev. 5-11/2006

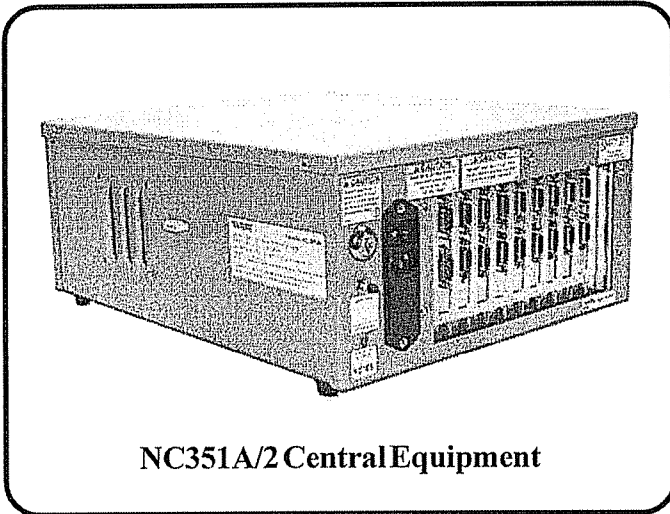

NC351A/2 Central Equipment

ARCHITECTS' AND ENGINEERS' SPECIFICATION

The nurse call central equipment shall be TekTone®'s NC351A or NC351A/2 or approved equal. The central equipment and associated wiring to master control stations and patient/staff stations shall be supervised. The central equipment shall include all necessary microprocessor multiplex-based circuitry to operate all Tek-CARE®NC300II system functions. It shall also support up to 4 (with NC351A) or 8 (with NC351A/2) nurses' master stations, plus 256 (with NC351A) or 512 (with NC351A/2) patient/staff stations, all associated lamp and other emergency and presence devices, and 2 isolated serial ports. The central equipment shall also provide the necessary firmware to operate all Tek-CARE®NC300II System functions.

The central equipment shall include one central buss board, one or two master interface cards, one microprocessor/serial card, one or two station interface cards, all call/multiplex card, multiple output power supply, and firmware operating system.

The central equipment will be housed in a durable metal enclosure with provisions for plug-in field wiring connections.

The NC351A and NC351A/2 shall be UL® 1069 Listed.

FEATURES

A major component of the Tek-CARE®NC300II Nurse Call System, the NC351A and NC351A/2 supply the central point for system component integration. The NC351A supports up to 4 master consoles and 256 station addresses, while the NC351A/2 supports up to 8 master consoles and 512 station addresses. The NC351A and NC351A/2 house the necessary firmware to operate all the Tek-CARE®NC300II system functions. From a single durable metal enclosure, the central equipment supports 2 isolated serial ports, field station ports, master console ports, and power requirements for up to 256 patient, staff and duty stations (512 with external PK305 Supply).

- UL® 1069 Listed
- 2 isolated serial ports
- Plug-in connections with multiplexed common wiring
- Self-contained electronics and power supply
- 12 or 24-hour time display
- Modular construction—easily expandable

SPECIFICATIONS

Dimensions:	19.5" × 15.5" × 5.25"
Capacity:	up to 4 (NC351A) or 8 (NC351A/2) masters, up to 256 (NC351A) or 512 (NC351A/2) stations
Power Input:	110–120V, 50–60Hz (internal jumper to switch to 220V)
Environments:	26°C, relative humidity maximum 80%
Terminations:	Plug-on connectors
System Supervision:	Continuous polling of all stations. Stations or wiring faults displayed at masters.
System Protection:	All outputs are protected by self-resetting current-limiting devices.
Audio:	Up to 4 (NC351A) or 8 (NC351A/2) audio paths provided. Amplifiers rated at 20 watts. Overload and short circuit protection included.

REQUIRED COMPONENTS

Tek-CARE®NC300II Nurse Call System


www.tektone.NET

277 Industrial Park Road • Franklin, NC 28734 • Phone (828) 524-9967 • Fax (828) 524-9968
Email: tektone@tektone.net • Technical Assistance Email: teksupt@tektone.net
TekTone®'s quality system is registered by UL® to the ISO 9001:2000 standard. (File #A10766.)



PK250A Power/Standby UPS Specification Sheet

IL472
Section E
Rev. 13-07/2006

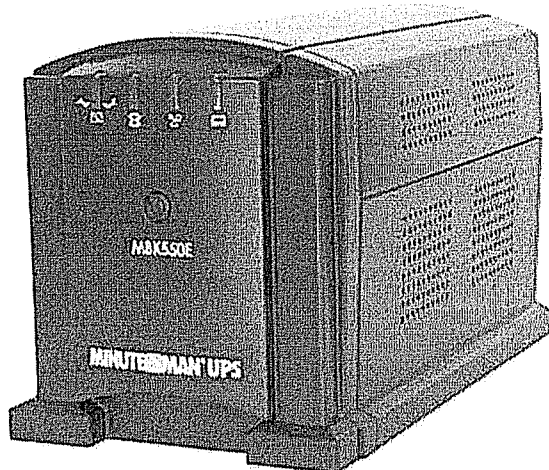

PK250A

ARCHITECTS' AND ENGINEERS' SPECIFICATION

The uninterruptible power supply shall be TekTone® PK250A or approved equal, and shall provide for continuous power in the event of utility power failures, brownouts, blackouts, or similar power interruptions.

The power supply shall have rugged construction and shall include power switch, audible alarm indicator, line output indicator, battery output indicator, output receptacles, power cord, and AC/DC fuses for utility power and battery protection.

The PK250A shall be UL® 1778 and CSA 22.1 Listed.

FEATURES

The PK250A Uninterruptable Power Supply is for use with TekTone's® Tek-CARE® NC300II Nurse Call System and provides uninterrupted power in the event of utility power failures, brownouts and blackouts. Its economical cost and compact size will enhance the operation of your system.

When power is interrupted, the PK250A immediately cuts in to provide square wave power for the Tek-CARE® NC300II Central Equipment until an emergency generator is activated or power is restored. In the event of a prolonged power outage, the PK250A will provide power to the limit of its battery. The green indicator on the front panel indicates power line output when steady, and battery output when flashing. The unit also provides an audible tone during battery output operation.

Other features include output receptacles for connection of equipment, power cord for standard 120 volt, 15 amp power circuit, AC fuses to protect the unit from utility power, and DC fuses to protect the battery.

- UL® 1778 and CSA 22.1 Listed.

SPECIFICATIONS

Output Rating

Wattage:	330 W
Voltage:	115 VAC
Frequency:	60 Hz
Waveform:	Stepped square wave

Input

Voltage:	115 VAC
Frequency:	60 Hz

Backup Operation

At full load:	5 min.
At half load:	15 min.
Transfer time:	2-6 ms typical

Battery

Type:	Maintenance-free 12 VDC 7Ah
Recharge:	8 hours
Auto cut-off:	Yes

Size

Overall:	8.65" × 9.0" × 8.5"
Weight:	18.8 lbs. (8.5 kg)
Operating temperature range is 0°C-40°C.	


www.tektone.NET

277 Industrial Park Road • Franklin, NC 28734 • Phone (828) 524-9967 • Fax (828) 524-9968
Email: tektone@tektone.net • Technical Assistance Email: teksupt@tektone.net
TekTone®'s quality system is registered by UL® to the ISO 9001:2000 standard. (File #A10766.)



PK305A Supplemental Power Supply Specification Sheet

IL698
Section E
Rev. 3-01/2006

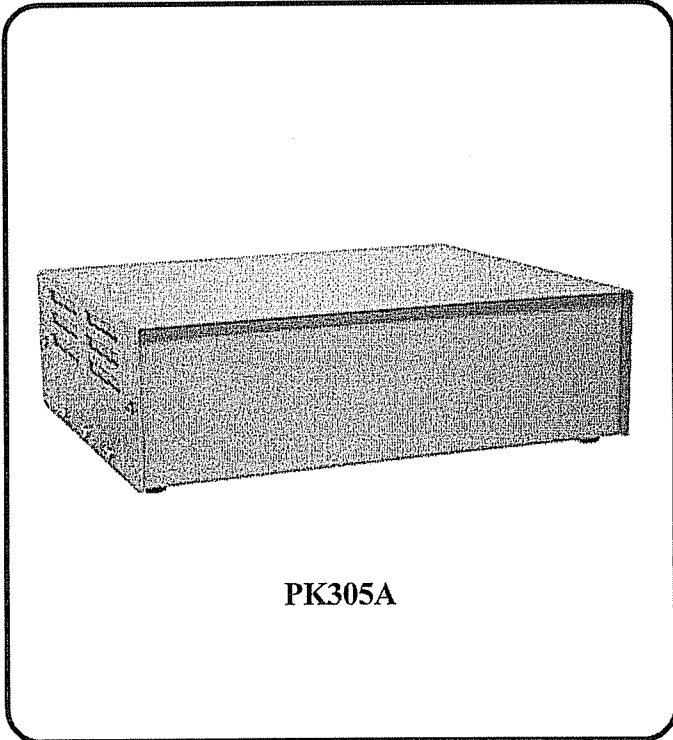

PK305A

ARCHITECTS' AND ENGINEERS' SPECIFICATION

The supplemental power supply shall be TekTone®'s PK305A or approved equal and will include the necessary hardware to interface with TekTone®'s NC351A/2 Central Equipment to provide additional power to support 512 stations.

The supplemental power supply will be housed in a durable metal enclosure with provisions for plug-in field wiring connections.

The supplemental power supply shall be UL® 1069 Listed.

FEATURES

The PK305A Supplemental Power Supply is used to provide additional power to the NC351A/2 Central Equipment to support 512 patient stations.

The supplemental power supply is housed in a durable metal enclosure with provisions for plug-in field wiring connections.

- Plug-in connectors for easy connection to NC351A/2 Central Equipment
- Provides additional power to the NC351A/2 Central Equipment to support 512 patient stations
- UL® 1069 Listed

SPECIFICATIONS

Dimensions:	Console: 10.75" x 8.75" x 3.25"
Power Input:	110-220V, 50-60Hz (internal jumper to switch to 220V)
Environments:	26°C, maximum 80% relative humidity
Terminations:	Plug-in connectors
System protection:	In-line fuses are provided on primary input

REQUIRED COMPONENTS

Tek-CARE®NC300II	Nurse Call System with NC351A/2 Central Equipment
------------------	---


www.tektone.NET

277 Industrial Park Road • Franklin, NC 28734 • Phone (828) 524-9967 • Fax (828) 524-9968
Email: tektone@tektone.net • Technical Assistance Email: teksupt@tektone.net
TekTone®'s quality system is registered by UL® to the ISO 9001:2000 standard. (File #A10766.)



SF401 Oxygen-Safe Call Cord Specification Sheet

IL767
Section E
Rev. 2 - 12/2005

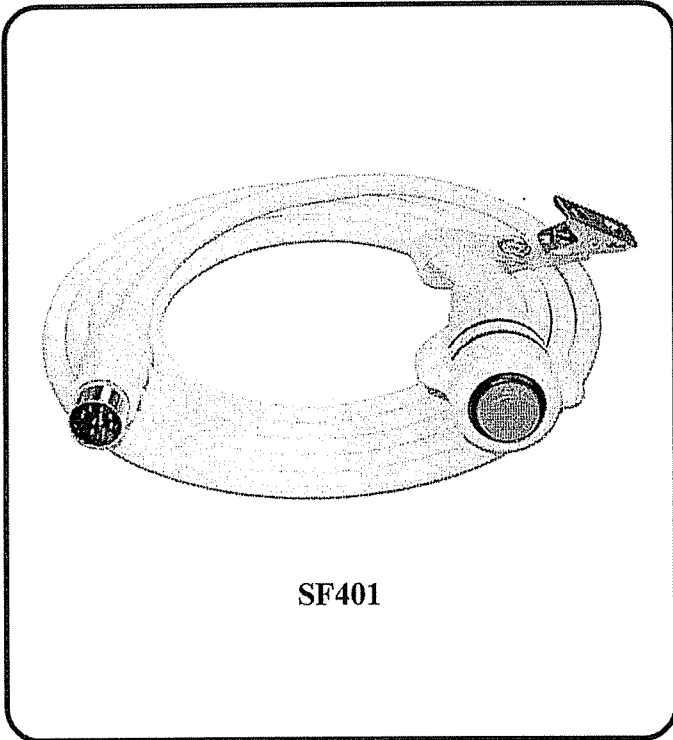

SF401

FEATURES

The TekTone® SF401 single call cord is for use with the Tek-CARE®NC300II nurse call system, where 8-pin DIN jacks are used. The SF401 is an oxygen safe call cord that is certified safe for use by all patients receiving oxygen therapy. This waterproof and impact resistant call cord has a completely sealed push button.

- UL® 1069 Listed
- Oxygen safe
- Impact resistant and waterproof
- Small, lightweight pendant fits comfortably in hand
- Bed clips included

SPECIFICATIONS

Connection: 8-pin DIN plug
 Construction: SPST1-A switch
 Integral brass, fine silver contacts
 1 AMP, 115 watt maximum, AC
 Dimensions: 7' (2.13 m) long polyvinyl-covered cord

REQUIRED COMPONENTS

Tek-CARE®NC300II	Nurse Call System
IR319/A or IR320/A	Patient Stations

ARCHITECTS' AND ENGINEERS' SPECIFICATION

Call cords shall be TekTone® SF401 or approved equal. Model SF401 shall provide one molded push button, shall be waterproof, and shall be suitable for use in oxygen environments.

The momentary-contact push button cordset shall be encased in a molded, shock-proof plastic shell. It shall be connected to a 7' (2.13 m) long polyvinyl covered cord with an integrally molded 8-pin DIN plug.

The SF401 shall be UL® 1069 Listed.


www.tektone.NET

277 Industrial Park Road • Franklin, NC 28734 • Phone (828) 524-9967 • Fax (828) 524-9968
 Email: tektone@tektone.net • Technical Assistance Email: teksupt@tektone.net
 TekTone®'s quality system is registered by UL® to the ISO 9001:2000 standard. (File #A10766.)



IR311E Single and IR312E Dual Patient Stations Specification Sheet

IL494
Section E
Rev. 7 - 12/2006

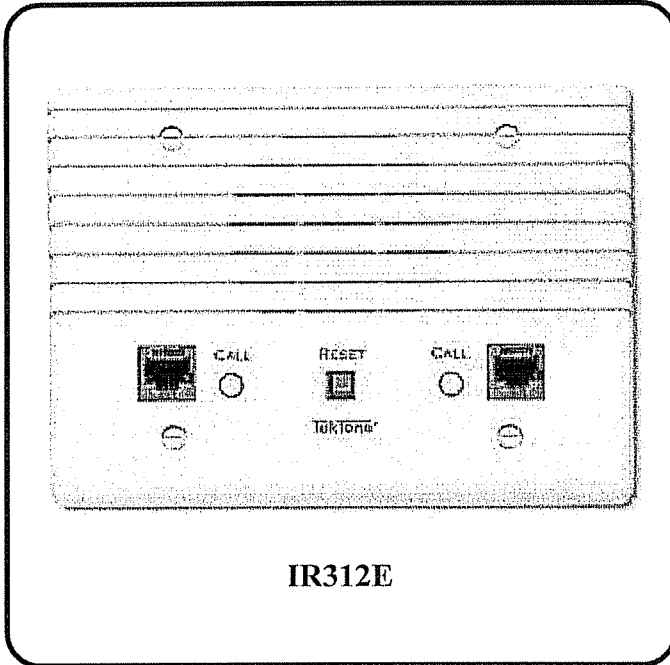

IR312E

ARCHITECTS' AND ENGINEERS' SPECIFICATION

Patient Stations shall be TekTone®'s IR311E, IR312E or approved equal. Stations, and wiring from the Central Equipment (CE) to stations, shall be supervised. The patient stations shall include solid-state LSI/microprocessor technology, yellow call-placed indicator(s), and combination red in-use indicator and reset button. Single patient stations shall include one 8-conductor modular RJ-45 jack type receptacle for pillow speakers or patient's call cord. Dual-patient stations shall include two jacks.

The station shall use a 2.5"×2.5" speaker/microphone for accurate voice reproduction. Removal of the call cord or pillow speaker from the receptacle shall result in placing a call with the indication of cord out at the master station. The call can be reset only by replacing the call cord or pillow speaker in its receptacle. All station components shall be mounted on an attractive, flame-retardant (UL® 94V-0) plastic panel. Connections shall be plug-in type.

The IR311E, IR312E shall be UL® 1069 Listed.

FEATURES

The IR311E Single Patient Station provides reliable two-way, hands-free communication between patient and nurse, and provides for programmable privacy, paging, and patient priority from the master station. Calling the nurse is accomplished by pressing the call cord button or the area indicated NURSE on the pillow speaker. Solid-state LEDs on the panel indicate the call has been placed and the intercom is in use. If the pillow speaker or call cord is accidentally removed from its receptacle, the nurse master station registers a non-cancelable call with cord out indication. The call may be reset only by returning the call cord or pillow speaker to its receptacle. The pillow speaker also provides television control.

The IR312E Dual Patient Station has the same specifications and functions as the IR311E, and has an additional independently operating call cord/pillow speaker receptacle, and another call-placed indicator.

- UL® 1069 Listed
- Fully supervised
- All stations interchangeable
- Simplified multiplex wiring & plug-in type connectors
- Input available for Hill-Rom® Sidecom® beds or remote call-in button applications
- Uses pillow speakers or push button call cords

SPECIFICATIONS

Dimensions:	Height:	4.5"	(114 mm)
	Width:	6.375"	(162 mm)
	Depth:	2.75"	(70 mm)
	Projects:	0.5"	(12.7 mm)
		above mounting surface	
Construction:	Flame-retardant (UL® 94V-0) plastic faceplate		
Speaker:	2.5"×2.5" (64 mm × 64 mm)		
Connections:	Plug-in type		
Housing:	Steel City #H3BD and #3GC plaster ring, or exact equal. Horizontal mount.		

REQUIRED COMPONENTS

Tek-CARE®NC300II Nurse Call System

www.tektone.NET

277 Industrial Park Road • Franklin, NC 28734 • Phone (828) 524-9967 • Fax (828) 524-9968


Email: tektone@tektone.net • Technical Assistance Email: teksupt@tektone.net

TekTone®'s quality system is registered by UL® to the ISO 9001:2000 standard. (File #A10766.)



IR315E Duty Station Specification Sheet

IL495
Section E
Rev. 9 - 11/2005

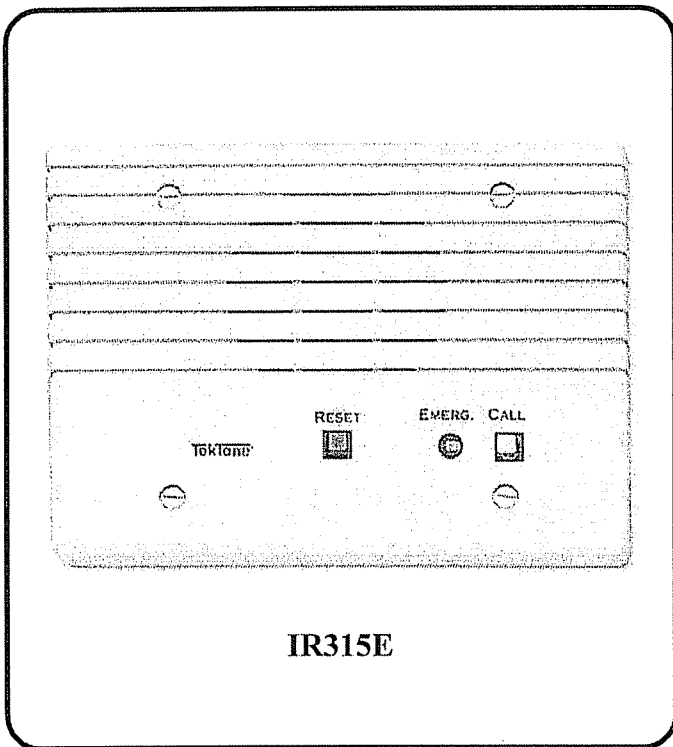

ARCHITECTS' AND ENGINEERS' SPECIFICATION

Duty station shall be TekTone® Model IR315E or approved equal. Model IR315E shall include solid-state LSI/Microprocessor technology, combination yellow call-placed indicator and call button, combination red in-use indicator and reset button, and red emergency/code call indicator. Audible and visual signaling of normal and emergency calls shall be provided. Three distinctive tone volume levels shall be available and shall be field-programmable at the station. It shall be possible, via user programming, to select the call priorities the duty station will annunciate. The station shall use a 2.5" x 2.5" speaker/microphone for accurate voice reproduction. All components shall be mounted on an attractive, flame retardant (UL® 94V-0) plastic panel. Connections shall be plug-in type.

The IR315E shall be UL® 1069 Listed.

FEATURES

The IR315E Duty Station provides reliable two-way, hands-free communication between the nurse master station and utility rooms, examination rooms, kitchen, or any location where a nurse may perform a function out of hearing or sight of the master station. Calls are placed to the master station by use of a momentary push button. When the call is answered at the master station, the red in-use indicator on the duty station lights, and the nurse may then carry on a conversation from the remote location.

A call originating from a patient station is indicated both audibly and visually at the duty station to which it is assigned. Normal calls are indicated by a steady illumination of the yellow call-placed indicator and a slow repeating tone. Emergency/bath calls cause alternate flashing of the yellow call-placed and red emergency indicators and a rapid repeating tone. Code calls function the same as emergency calls, but at twice the pulse rate. Dome light indication is also provided. All calls initiated from stations other than the duty station can be reset only at the master station or point of origin.

- UL® 1069 Listed
- Supervised
- All stations interchangeable
- Simplified multiplex wiring using plug-in connectors
- Attractive, flame retardant (UL® 94V-0) plastic faceplate
- Selective annunciation of call priority

SPECIFICATIONS

Dimensions:	Height:	4.5"	(114 mm)
	Width:	6.375"	(162 mm)
	Depth:	2.75"	(70 mm)
	Projects:	0.5"	(12.7 mm)
Construction:	Flame retardant (UL® 94V-0) plastic		
Speaker:	2.5" x 2.5" (64 mm x 64 mm), 60 ohm		
Connections:	Plug-in type		
Housing:	Steel City #H3BD with Steel City #3GC plaster ring, or exact equal. Horizontal mount.		

REQUIRED COMPONENTS

Tek-CARE®NC300II Nurse Call System


www.tektone.NET

277 Industrial Park Road • Franklin, NC 28734 • Phone (828) 524-9967 • Fax (828) 524-9968
Email: tektone@tektone.net • Technical Assistance Email: teksupt@tektone.net
TekTone®'s quality system is registered by UL® to the ISO 9001:2000 standard. (File #A10766.)



LI386B Addressable Dome/Zone Light Specification Sheet

IL547
Section E
Rev. 9 - 11/2005

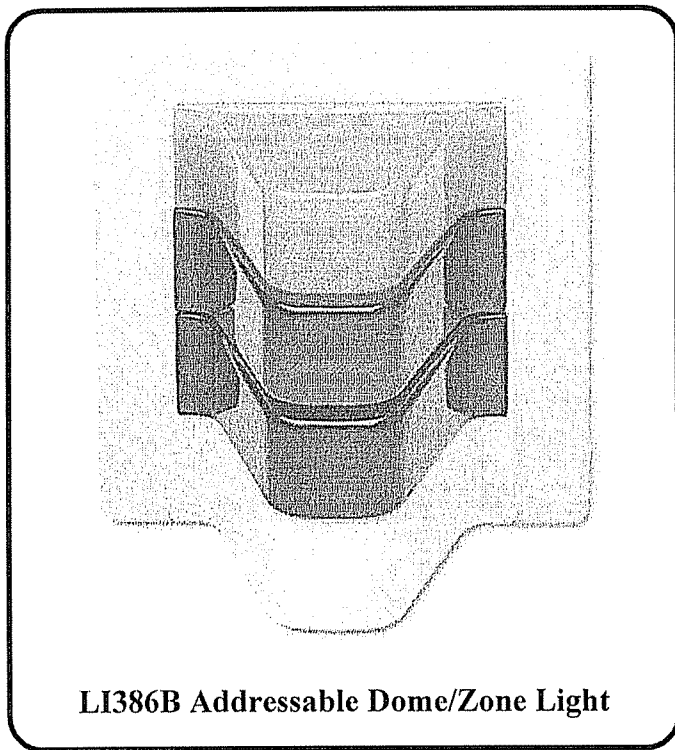

LI386B Addressable Dome/Zone Light

ARCHITECTS' AND ENGINEERS' SPECIFICATION

Dome/Zone light shall be TekTone® LI386B or approved equal. The supervised corridor light shall be sectional in design. Lights shall include one each amber, red and green flame-retardant translucent polycarbonate plastic lenses, and one white flame-retardant translucent polystyrene plastic lens. All lenses shall be mounted on a flame-retardant (UL® 94V-0) plastic base panel. The lenses shall be individually removable without the use of tools, for ease of bulb replacement. The four bulbs, in conjunction with the different colored lenses, shall provide for indication of patient call priority and staff presence. The Dome/Zone light shall have lamp supervision.

The stations, and the wiring from the central equipment (CE) to the stations, shall be supervised. The unit shall provide visual and digital communications to and from the CE. Connections shall be plug-in type. The LI386B shall be a stand-alone unit that connects directly to the CE.

The Dome/Zone light shall be UL® 1069 Listed.

FEATURES

TekTone®'s LI386B Dome/Zone Light with built-in multipurpose station provides visual indication of calls originating from bath, emergency and code call stations when used as a dome light. The LI386B also indicates calls originating from patient, staff and duty stations when used as a zone light. The LI386B also indicates all calls from the zones to which those stations are assigned and provides communication to and from the central equipment, including the nurse master station and monitor. It is used with remotely-mounted devices such as switches, contact closures, or other signal-originating equipment. No controls are provided.

- UL® 1069 Listed
- Supervised
- Easy bulb replacement
- Excellent visibility
- Lamp supervision
- Interchangeable lens caps
- Simplified multiplex wiring
- Plug-in connectors

SPECIFICATIONS

Dimensions:	Height: 4.5625" (115 mm)
	Width: 4.5625" (115 mm)
	Depth: 3.3" (84 mm)
Bulbs:	#1829 28v. 70mA
Power:	24 VDC, 51 mA
Connections:	Ramp lock plug-in type
Finish:	Base is flame retardant (UL® 94V-0) plastic. Amber, red and green lenses are flame-retardant translucent polycarbonate plastic. White lens is flame retardant translucent polystyrene plastic.
Housing:	Standard dual gang box and ring.

REQUIRED COMPONENTS

Tek-CARE®NC300II Nurse Call System


www.tektone.NET

277 Industrial Park Road • Franklin, NC 28734 • Phone (828) 524-9967 • Fax (828) 524-9968
Email: tektone@tektone.net • Technical Assistance Email: teksupt@tektone.net
TekTone®'s quality system is registered by UL® to the ISO 9001:2000 standard. (File #A10766.)



SF341B Code Call Station Specification Sheet

IL510
Section E
Rev. 12 - 11/2005

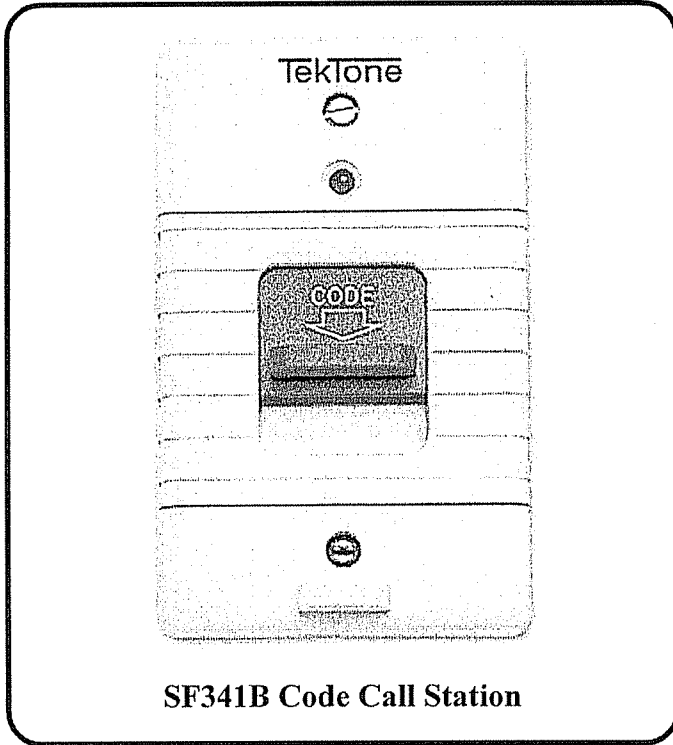

SF341B Code Call Station

FEATURES

The SF341B Code Call Station operates all system code signals, and is designed for use in ICU/CCU, physical therapy rooms, post-op recovery, or any location where code call initiation may be required. The large 1.1" (28 mm) blue pull-down lever is used for code call activation. The red call-placed LED indicator flashes to provide for call assurance. Calls are registered on the master station (and duty station, if used) via audible and visual signals pulsing at a rate of twice that of a standard emergency signal. Local indication on dome lights is also provided. Call cancellation is possible only at the originating location.

- UL® 1069 Listed
- Supervised
- Registers audible and visual calls at master station
- Indicates local call origination on dome lights
- Simple and flexible operation
- Call-placed indicator
- Call cancel at point of origin
- Flame retardant (UL® 94V-0) plastic faceplate
- 1.1" (28 mm) wide pull-down lever

ARCHITECTS' AND ENGINEERS' SPECIFICATION

Code call station shall be TekTone® SF341B or approved equal. Code stations and wiring from code stations to patient stations shall be supervised. Operation of code signals shall be accomplished by pulling down on the blue lever marked CODE.

The red call-placed LED indicator shall flash to assure that the call has been properly placed. The initiation of the code call shall cause the activation of both audible and visual signals, pulsing at a rate twice that of a standard emergency signal. Call cancellation shall be possible only at point of origin. Reliable, solid-state components shall be used, and plug-in connectors shall be provided for electrical connections.

The SF341B shall be UL® 1069 Listed.

SPECIFICATIONS

Dimensions:	Height:	4.50" (114 mm)
	Width:	2.8125" (72 mm)
	Depth:	1.625" (41 mm)
	Projects:	0.6875" (17 mm)
		from mounting surface (including pull down lever)
Construction:	Flame retardant (UL® 94V-0) plastic faceplate. Switch and electronic components are circuit board mounted.	
Connections:	Plug-in connectors.	
Housing:	Single gang ring (IH357) with square box (IH358), or exact equal.	

REQUIRED COMPONENTS

Tek-CARE®NC300II Nurse Call System


www.tektone.NET

277 Industrial Park Road • Franklin, NC 28734 • Phone (828) 524-9967 • Fax (828) 524-9968
Email: tektone@tektone.net • Technical Assistance Email: teksupt@tektone.net
TekTone®'s quality system is registered by UL® to the ISO 9001:2000 standard. (File #A10766.)



SF337C Emergency Shower Switch Specification Sheet

IL629
Section E
Rev. 8-02/2006

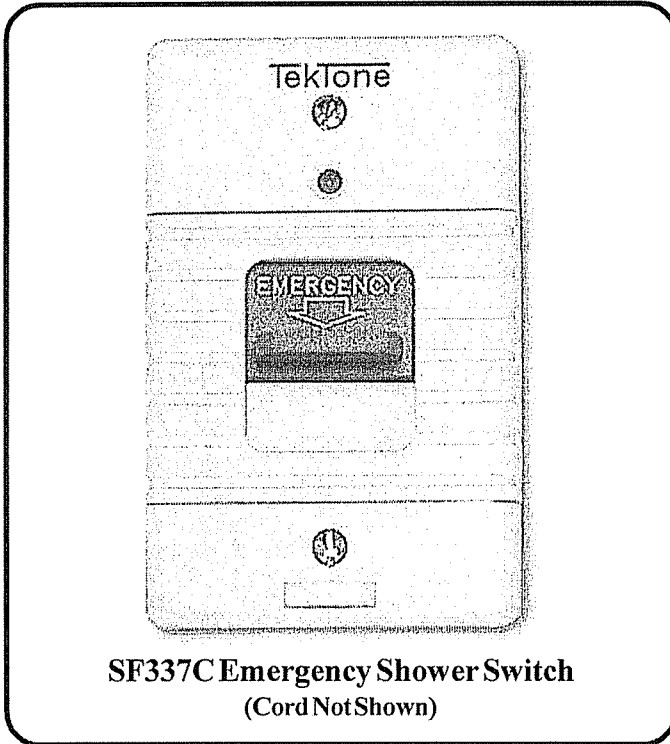

SF337C Emergency Shower Switch
(Cord Not Shown)

ARCHITECTS' AND ENGINEERS' SPECIFICATION

The emergency shower switch shall be TekTone® SF337C or approved equal. Operation of emergency signals shall be accomplished by a short pull on the nylon cord or by pulling down on the RED lever marked EMERGENCY.

The red CALL-PLACED indicator shall flash to assure the patient that the call has been placed.

The emergency shower switch shall be waterproof if mounted according to manufacturer's instructions. If mounted correctly, the faceplate shall be sealed from the electronic components. The switching mechanism shall consist of a reliable reed switch with a sealed magnet actuator.

The SF337C shall be UL® 1069 Listed.

FEATURES

The SF337C Emergency Shower Switch is for any location where activation of an emergency signal is required. The design is such that it may be located anywhere in a shower, bath or tub room, regardless of environmental conditions. The combination of rubber-grommetted mounting screws, rubber mounting gasket, and completely sealed front faceplate make it waterproof (if properly installed). Electronic components are mounted on a circuit board, including an industry-proven reliable reed switch for circuit initiation. The activating magnet is mounted on the large pull-down lever, which is completely sealed in plastic. The indicator LED is also completely sealed.

Due to the flexibility of its design, the SF337C may be used as a pull cord or as a pull down activated emergency switch. The pull cord supplied may be used for emergency call activation, or if desired, the large 1.1" (28mm) red pull-down lever may be used. Dome light and system annunciation vary according to the manner in which the SF337C is connected.

- UL® 1069 Listed
- Waterproof—if installed according to manufacturer's instructions
- Call-placed indicator
- Call cancel at point of origin
- Attractive, flame-retardant (UL® 94V-0) plastic faceplate
- 1.1" (28mm) wide pull-down lever

SPECIFICATIONS

Dimensions:	Height:	4.5"	(114mm)
	Width:	2.8125"	(72 mm)
	Depth:	1.625"	(41 mm)
	Projects:	0.6875"	(17 mm)
		(including pull down lever)	
Construction:	Flame-retardant (UL® 94V-0) plastic		
Connections:	Plug-in type.		
Housing:	Single gang ring with square box.		

REQUIRED COMPONENTS

Tek-CARE® NC300II,
NC200, NC150, NC110 Nurse Call Systems
or
Tek-CARE® 500 Wireless Emergency Call System

www.tektone.NET

277 Industrial Park Road • Franklin, NC 28734 • Phone (828) 524-9967 • Fax (828) 524-9968
Email: tektone@tektone.net • Technical Assistance Email: teksupt@tektone.net
TekTone®'s quality system is registered by UL® to the ISO 9001:2000 standard. (File #A10766.)