



State of West Virginia  
 Department of Administration  
 Purchasing Division  
 2019 Washington Street East  
 Post Office Box 50130  
 Charleston, WV 25305-0130

# Request for Quotation

RFO NUMBER  
**EHP11097**

PAGE  
**1**

ADDRESS CORRESPONDENCE TO ATTENTION OF  
**ROBERTA WAGNER**  
**304-558-0067**

VENDOR

RFQ COPY  
 TYPE NAME/ADDRESS HERE

*Source-Ray, Inc.*  
*50 Fleetwood Court*  
*Ronkonkoma, NY 11779*

SHIP TO

**HEALTH AND HUMAN RESOURCES**  
**BPH - TUBERCULOSIS CONTROL**  
**350 CAPITOL STREET, ROOM 125**  
**CHARLESTON, WV**  
**25301-3715 304-558-3669**

DATE PRINTED <b>11/29/2010</b>	TERMS OF SALE	SHIP VIA	F.O.B.	FREIGHT TERMS
BID OPENING DATE: <b>12/30/2010</b>		BID OPENING TIME <b>01:30PM</b>		

LINE	QUANTITY	UOP	CAT. NO.	ITEM NUMBER	UNIT PRICE	AMOUNT
001	2	EA		898-80	\$ 18,525.00	\$ 37,050.00
<p><i>Source-Ray, Inc.</i></p> <p><b>MINXRAY HP 120/60HPPWV POWER PLUS, OR EQUAL, HIGH EQUIVALENT MODEL POWER MAX 1260 HIGH FREQUENCY PORTABLE X-RAY SYSTEM INCLUDING 1260 MOBILE STAND.</b></p> <p><b>FREQUENCY PORTABLE MEDICAL X-RAY UNIT, PER THE ATTACHED SPECIFICATIONS.</b></p> <p><b>CANCELLATION: THE DIRECTOR OF PURCHASING RESERVES THE RIGHT TO CANCEL THIS CONTRACT IMMEDIATELY UPON WRITTEN NOTICE TO THE VENDOR IF THE COMMODITIES AND/OR SERVICE SUPPLIED ARE OF AN INFERIOR QUALITY OR DO NOT CONFORM TO THE SPECIFICATIONS OF THE BID AND CONTRACT HEREIN.</b></p> <p><b>BANKRUPTCY: IN THE EVENT THE VENDOR/CONTRACTOR FILES FOR BANKRUPTCY PROTECTION, THE STATE MAY DEEM THE CONTRACT NULL AND VOID, AND TERMINATE SUCH CONTRACT WITHOUT FURTHER ORDER.</b></p> <p><b>INQUIRIES: WRITTEN QUESTIONS SHALL BE ACCEPTED THROUGH CLOSE OF BUSINESS ON 12/14/2010. QUESTIONS MAY BE SENT VIA USPS, FAX, COURIER OR E-MAIL. IN ORDER TO ASSURE NO VENDOR RECEIVES AN UNFAIR ADVANTAGE, NO SUBSTANTIVE QUESTIONS WILL BE ANSWERED ORALLY. IF POSSIBLE, E-MAIL QUESTIONS ARE PREFERRED. ADDRESS INQUIRIES TO:</b></p> <p><b>ROBERTA WAGNER</b>  <b>DEPARTMENT OF ADMINISTRATION</b>  <b>PURCHASING DIVISION</b>  <b>2019 WASHINGTON STREET, EAST</b>  <b>CHARLESTON, WV 25311</b></p> <p style="text-align: right;"><b>RECEIVED</b>  <b>DEC 29 A 8:41</b></p>						

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE: *R. M...* TELEPHONE: **631-244-8200** DATE: **12/28/10**

TITLE: *President* FEIN: **26-0011212**

ADDRESS CHANGES TO BE NOTED ABOVE

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED 'VENDOR'



State of West Virginia  
 Department of Administration  
 Purchasing Division  
 2019 Washington Street East  
 Post Office Box 50130  
 Charleston, WV 25305-0130

# Request for Quotation

RFQ NUMBER  
**EHP11097**

PAGE  
**2**

ADDRESS CORRESPONDENCE TO ATTENTION OF  
**ROBERTA WAGNER**  
**304-558-0067**

RFQ COPY

TYPE NAME/ADDRESS HERE

*Source-Ray, INC.*  
*50 Fleetwood Court*  
*Roxbury, MA, NY 11779*

SHIP TO

HEALTH AND HUMAN RESOURCES  
 BPH - TUBERCULOSIS CONTROL  
 350 CAPITOL STREET, ROOM 125  
 CHARLESTON, WV  
 25301-3715 304-558-3669

DATE PRINTED	TERMS OF SALE	SHIP VIA	FOB	FREIGHT TERMS
11/29/2010				
BID OPENING DATE: 12/30/2010		BID OPENING TIME 01:30PM		

LINE	QUANTITY	UOP	CAT NO	ITEM NUMBER	UNIT PRICE	AMOUNT
<p>FAX: 304-558-4115            E-MAIL: ROBERTA.A.WAGNER@WV.GOV</p> <p>THE MODEL/BRAND/SPECIFICATIONS NAMED HEREIN ESTABLISH THE ACCEPTABLE LEVEL OF QUALITY ONLY AND ARE NOT INTENDED TO REFLECT A PREFERENCE OR FAVOR ANY PARTICULAR BRAND OR VENDOR. VENDORS WHO ARE BIDDING ALTERNATES SHOULD SO STATE AND INCLUDE PERTINENT LITERATURE AND SPECIFICATIONS. FAILURE TO PROVIDE INFORMATION FOR ANY ALTERNATES MAY BE GROUNDS FOR REJECTION OF THE BID. THE STATE RESERVES THE RIGHT TO WAIVE MINOR IRREGULARITIES IN BIDS OR SPECIFICATION IN ACCORDANCE WITH SECTION 148-1-4(F) OF THE WEST VIRGINIA LEGISLATIVE RULES AND REGULATIONS.</p> <p>VENDOR PREFERENCE CERTIFICATE</p> <p>THIS TEAM EXHIBIT HAS BEEN REPLACED BY THE ONLINE VERSION WHICH IS AVAILABLE HERE:  <a href="http://www.state.wv.us/admin/purchase/vrc/venpref.pdf">HTTP://WWW.STATE.WV.US/ADMIN/PURCHASE/VRC/VENPREF.PDF</a></p> <p>NOTICE</p> <p>A SIGNED BID MUST BE SUBMITTED TO:</p> <p>DEPARTMENT OF ADMINISTRATION            PURCHASING DIVISION            BUILDING 15            2019 WASHINGTON STREET, EAST            CHARLESTON, WV 25305-0130</p>						

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE: *R. Mary* TELEPHONE: **631-244-8200** DATE: **12/28/10**

TITLE: *President* FEIN: **26-0011212** ADDRESS CHANGES TO BE NOTED ABOVE

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED 'VENDOR'



State of West Virginia  
 Department of Administration  
 Purchasing Division  
 2019 Washington Street East  
 Post Office Box 50130  
 Charleston, WV 25305-0130

# Request for Quotation

RFQ NUMBER
EHP11097

PAGE
3

ADDRESS CORRESPONDENCE TO ATTENTION OF
ROBERTA WAGNER 304-558-0067

VENDOR

RFQ COPY  
 TYPE NAME/ADDRESS HERE

Source-Ray, INC.  
 50 Fleetwood Court  
 Ronkonkoma, NY 11779

SHIP TO

HEALTH AND HUMAN RESOURCES  
 BPH - TUBERCULOSIS CONTROL  
 350 CAPITOL STREET, ROOM 125  
 CHARLESTON, WV  
 25301-3715 304-558-3669

DATE PRINTED	TERMS OF SALE	SHIP VIA	F.O.B.	FREIGHT TERMS
11/29/2010				

BID OPENING DATE: 12/30/2010 BID OPENING TIME 01:30PM

LINE	QUANTITY	UOP	CAT NO	ITEM NUMBER	UNIT PRICE	AMOUNT
<p>THE BID SHOULD CONTAIN THIS INFORMATION ON THE FACE OF THE ENVELOPE OR THE BID MAY NOT BE CONSIDERED:</p> <p>SEALED BID</p> <p>BUYER: -----RW/FILE 22-----</p> <p>RFQ. NO.: -----EHP11097-----</p> <p>BID OPENING DATE: -----12/30/2010-----</p> <p>BID OPENING TIME: -----1:30 PM-----</p> <p>PLEASE PROVIDE A FAX NUMBER IN CASE IT IS NECESSARY TO CONTACT YOU REGARDING YOUR BID:</p> <p>-----Source-Ray INC. Fax # (631) 244-7464-----</p> <p>CONTACT PERSON (PLEASE PRINT CLEARLY):</p> <p>-----Ray MAHEZ, (631) 244-8200 x302-----</p>						
0002	2	EA	898-80		N/A	N/A
<p>MINXRAY XGS MKIV LW, OR EQUAL, PORTABLE MOBILE STAND</p> <p>Source-Ray Powermax 1260 Includes mobile stand</p>						

PER THE ATTACHED SPECIFICATIONS TERMS AND CONDITIONS

SIGNATURE R. Alamy	TELEPHONE 631-244-8200	DATE 12/28/10
TITLE President	FEIN 26-0011212	ADDRESS CHANGES TO BE NOTED ABOVE

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED 'VENDOR'



State of West Virginia  
 Department of Administration  
 Purchasing Division  
 2019 Washington Street East  
 Post Office Box 50130  
 Charleston, WV 25305-0130

# Request for Quotation

RFQ NUMBER  
 EHP11097

PAGE  
 4

ADDRESS CORRESPONDENCE TO ATTENTION OF  
 ROBERTA WAGNER  
 304-558-0067

VENDOR

RFQ COPY  
 TYPE NAME/ADDRESS HERE

Source-Ray, Inc.  
 50 Fleetwood Court  
 Ron Kon Koma, NY 11774

SHIP TO

HEALTH AND HUMAN RESOURCES  
 BPH - TUBERCULOSIS CONTROL  
 350 CAPITOL STREET, ROOM 125  
 CHARLESTON, WV  
 25301-3715 304-558-3669

DATE PRINTED	TERMS OF SALE	SHIP VIA	F.O.B.	FREIGHT TERMS
11/29/2010				

BID OPENING DATE: 12/30/2010 BID OPENING TIME 01:30PM

LINE	QUANTITY	UOP	CAT NO	ITEM NUMBER	UNIT PRICE	AMOUNT
***** THIS IS THE END OF RFQ EHP11097 ***** TOTAL:						\$ 31,050.00

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE R. Henry TELEPHONE 631-244-8200 DATE 12/28/10  
 TITLE President FEIN 26-001212  
 ADDRESS CHANGES TO BE NOTED ABOVE

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED 'VENDOR'

**Portable x-ray unit must include the following:**

Unit must produce 40-120 KVDC, over 200 MAS and variable MA (60-20).

Unit must be complete with CPU control, high resolution timer, adjustable light beam collimator, power cord, exposure cord and technique chart for 100-260V AC, 50/60HZ use.

Unit must have 5 memory stations to store and easily recall frequently used exposure techniques.

Weight of unit must not exceed 50 pounds.

**Mobile stand must include the following:**

Stand must be stainless steel with 16" wheels.

Weight of stand must not exceed 50 pounds.

X-ray unit and stand must be heavy duty. Total weight of unit and stand must not exceed 100 pounds.

Inside delivery required (no trade-ins).

COST SHEET FOR EHP11097

Item #	App. Annual Usage	Description	Unit Price	Total Cost
1	2 each	Source-Ray Power Man 1260 <del>Min X-ray HF 120 60HP Power Plus</del> High Frequency Portable Medical X-ray Unit (for equal) <i>including mobile stand</i>	\$ 18,525.00	\$ 37,050.00
2	2 each	Min X-ray XGS MIKIV LW Portable Mobile Stand (for equal)	N/A	N/A
3	1 each	Shipping (if applicable) Source-Ray Price Quoted FOB Destination		
TOTAL COST				

Award will be made to the vendor with the lowest overall cost who meets specifications.

Vendor shall deliver within thirty days of purchase order receipt.

A minimum one year warranty is required.

Vendor must submit an original itemized invoice for order. Payment will be made in arrears after receipt of completed order.

RFQ No. EHP 11097

STATE OF WEST VIRGINIA  
Purchasing Division

**PURCHASING AFFIDAVIT**

**West Virginia Code §5A-3-10a states:** No contract or renewal of any contract may be awarded by the state or any of its political subdivisions to any vendor or prospective vendor when the vendor or prospective vendor or a related party to the vendor or prospective vendor is a debtor and the debt owed is an amount greater than one thousand dollars in the aggregate.

**DEFINITIONS:**

"Debt" means any assessment, premium, penalty, fine, tax or other amount of money owed to the state or any of its political subdivisions because of a judgment, fine, permit violation, license assessment, defaulted workers' compensation premium, penalty or other assessment presently delinquent or due and required to be paid to the state or any of its political subdivisions, including any interest or additional penalties accrued thereon.

"Debtor" means any individual, corporation, partnership, association, limited liability company or any other form or business association owing a debt to the state or any of its political subdivisions. "Political subdivision" means any county commission; municipality; county board of education; any instrumentality established by a county or municipality; any separate corporation or instrumentality established by one or more counties or municipalities, as permitted by law; or any public body charged by law with the performance of a government function or whose jurisdiction is coextensive with one or more counties or municipalities. "Related party" means a party, whether an individual, corporation, partnership, association, limited liability company or any other form or business association or other entity whatsoever, related to any vendor by blood, marriage, ownership or contract through which the party has a relationship of ownership or other interest with the vendor so that the party will actually or by effect receive or control a portion of the benefit, profit or other consideration from performance of a vendor contract with the party receiving an amount that meets or exceed five percent of the total contract amount.

**EXCEPTION:** The prohibition of this section does not apply where a vendor has contested any tax administered pursuant to chapter eleven of this code, workers' compensation premium, permit fee or environmental fee or assessment and the matter has not become final or where the vendor has entered into a payment plan or agreement and the vendor is not in default of any of the provisions of such plan or agreement.

Under penalty of law for false swearing (*West Virginia Code §61-5-3*), it is hereby certified that the vendor affirms and acknowledges the information in this affidavit and is in compliance with the requirements as stated.

**WITNESS THE FOLLOWING SIGNATURE**

Vendor's Name: Source-Ray, Inc.

Authorized Signature: Raymond Henry Date: 12/28/10

State of New York

County of Suffolk, to-wit:

Taken, subscribed, and sworn to before me this 28<sup>th</sup> day of December, 2010.

My Commission expires 09-04, 2013

**AFFIX SEAL HERE**

ELAYNE GRECO NOTARY PUBLIC Elayne Greco  
Notary Public - State of New York  
No. 01GR6063623  
Qualified in Suffolk County  
My Commission Expires 09/04/2013




# POWERMAX 1260

**sri**  
source-ray, inc.



- Maximum Power Output
- 3.0 kW Across Full Range
- 120 kV, 15 – 60 mA
- High Frequency - Power Factor Correction
- Universal Input Voltage
- Microprocessor Control
- CR/DR Compatible
- Light Weight
- Designed for Reliability
- Durable Powder Coat Finish
- Limited 3 year warranty

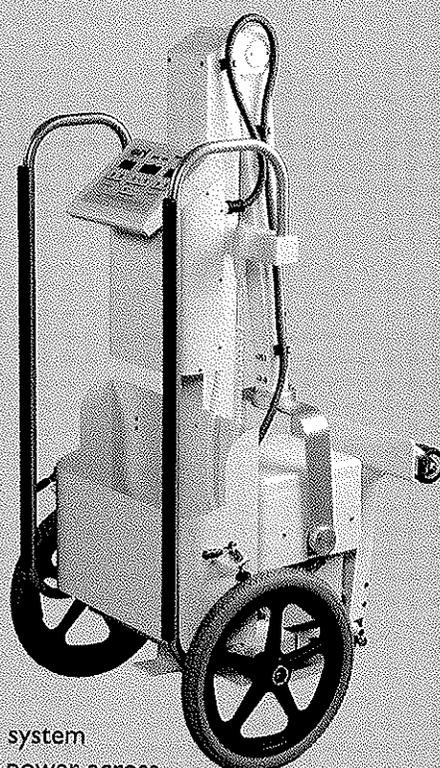

**PowerMax 1260** Provides maximum power, state of the art technology, system reliability and low maintenance, all in a small footprint, lightweight package.

The **PowerMax 1260** was designed with agility in mind.

Its compact, lightweight construction makes it easy for the operator to move the system effortlessly. Delivering maximum mR/mAs, the PowerMax 1260 produces 3kW of power across the entire kV range. With its constant 3kW output, the **PowerMax 1260** provides hospital quality imaging and offers an easy upgrade path for clinical sites transitioning to Digital Imaging.

The **PowerMax 1260** provides the power required to compensate for the slower operating speeds of CR Systems, and is the ideal **High Power portable x-ray system** for organizations considering the purchase of CR Systems.

The **PowerMax 1260** is suitable for use in Hospitals, Urgent Care Facilities, Medical Examiner Offices, Nursing Homes, Home Healthcare, Orthopedic Practices, Sports Medicine, Correctional Facilities, and Military Field Deployable Applications.

See why Source-Ray continues to set the Standard for **Quality Portable Imaging Solutions**.

**Source-Ray, Inc.**

# POWERMAX 1260 ELECTRICAL SPECIFICATIONS

## Generator

Power 3.0 kW across full range  
 Input Voltage 110 - 230 VAC 50/60 Hz  
 kVp Range 40 - 120 kVp, adjustable in 1 kV increments - Closed loop regulation  
 Power Factor Correction

mA Range Adjustable, 15 mA - 60 mA - closed loop regulation

mAs Range 0.125 - 200  
 Exposure Time 0.01 - 3.33 seconds  
 Indicators Digital display of kVp, mAs and Exposure Time X-Ray, Ready, mA Station and Fault Indicators.

Filtration 3.6 mm al minimum @ 100kVp  
 4.3 mm al minimum @ 120kVp

Exposure Switch Detachable two-position

## X-Ray Tube

Target Material Stationary Anode 130 kVp  
 Tungsten  
 Anode Capacity 30,000 HU Storage  
 Focal Spot 1.2 mm  
 Target Angle 15°

## Collimator

Laser Crosshairs  
 Tape Measure  
 Inclinator  
 Collimate CP-100-24-C  
 Center Locator  
 SID Measurement  
 Angle Measurement


## Model SR-1260

### Travel Stand

Min. F/S to Floor 13" / 33 cm  
 Max. F/S to Floor 78" / 198 cm  
 Hor. Ext. of F/S 21" / 53 cm  
 Hor. Rotation 200°  
 Tube Rotation 270°

### System Weight




110 lbs. / 45 kg

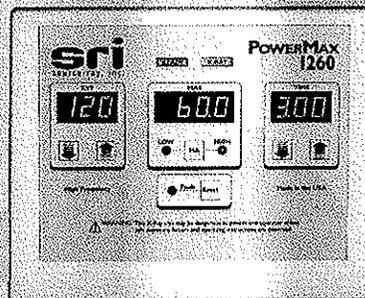

Complies with CFR 21 subchapter J



## DIAGRAMS

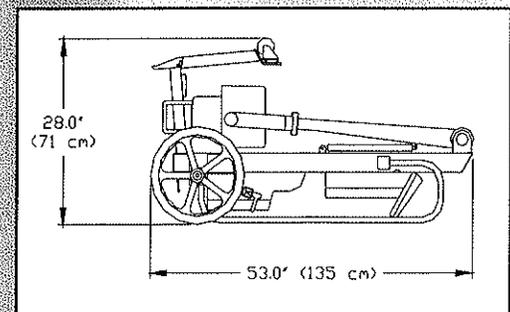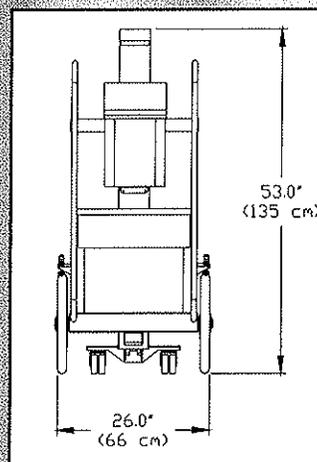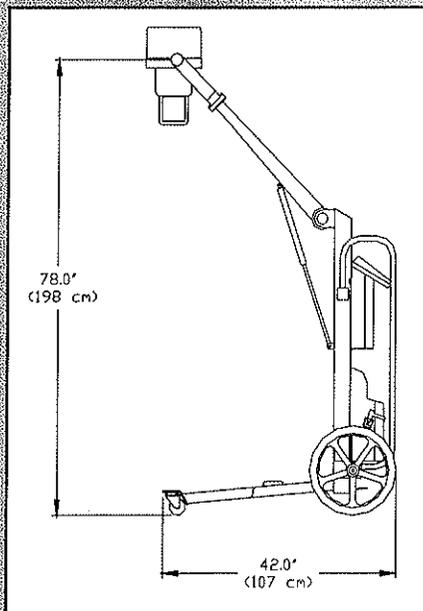

**sri**  
 source-ray, inc.

Specifications are subject to change without notice.

Source-Ray, Inc. • 167 Keyland Court • Bohemia, NY 11716  
 (631) 244-8200 • Email: x\_raysales@sourceray.com • fax (631) 244-7464





## Limited Three Year Warranty

*(Film Based Portable Systems)*

**Source-Ray, Inc.** warrants its Model **SR-115, SR-130 and PowerMax 1260**

Portable X-Ray Systems to be free of manufacturing defects, which can impair their normal operation when used within their specified ratings. Claims under this warranty must be made within 3 years after shipment from the factory. Such warranty shall not apply to defects resulting from accidents, alterations, abuse or misuse. X-Ray Tube and Collimator warranty is limited to that provided by the manufacturer. Liability under this warranty is limited to repair or replacement of defective components at the factory. **Shipping costs are not included.** This warranty is in lieu of any other warranty expressed or implied. Collimator bulbs, exposure and line cord assemblies, interconnect cables and tires are considered normal wear and tear and are not covered under this limited warranty.

**Source-Ray, Inc.**

50 Fleetwood Ct., Ronkonkoma NY 11779

631-244-8200