



State of West Virginia
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Post Office Box 50130
 Charleston, WV 25305-0130

Request for Quotation

RFQ NUMBER
LBS12015

PAGE
1

ADDRESS CORRESPONDENCE TO ATTENTION OF:
ROBERTA WAGNER 304-558-0067

VENDOR

*506084009 800-426-8157
 QIAGEN INC
 27220 TURNBERRY LANE STE 200
 VALENCIA CA 91355-1005

SHIP TO

HEALTH AND HUMAN RESOURCES
 BPH - LABORATORY SERVICES
 167-ELEVENTH AVENUE
 SOUTH CHARLESTON, WV
 25303 304-558-3530

DATE PRINTED	TERMS OF SALE	SHIP VIA	F.O.B.	FREIGHT TERMS
08/15/2011	NET 30	UPS or OTHER	SHIPPING POINT	PREPAID & ADDED

BID OPENING DATE: 09/15/2011 CARRIER PER BID OPENING TIME 01:30PM

LINE	QUANTITY	UOP	CAT. NO.	ITEM NUMBER	UNIT PRICE	AMOUNT
0001	1	JB		193-36		
<p>AUTOMATED NUCLEIC ACID PURIFICATION SYSTEM</p> <p>TO PROVIDE A MAGNA PURE COMPACT SYSTEM, OR EQUAL, TO PERFORM FAST AND EASY AUTHOMATION OF NUCLEIC ACID PURIFICATION FROM UNKNOWN ENVIRONMENTAL SAMPLES DURING A BIOTERRORISM EVENT. THE SYSTEM MINIMIZES CONTAMINATION RISK WITH PREFILLED REAGENTS AND DISPOSABLES, SYNCHRONIZED STAGE MOVEMENT, AN INTEGRATED HEPA FILTER AND UV DECONTAMINATION WHICH IS VERY CRITICAL WHEN DEALING WITH SUSPECT BIOTERRORISM SAMPLES, PER THE ATTACHED SPECIFICATIONS.</p> <p>EQUIPMENT MUST BE FDA APPROVED.</p> <p>SHIPPING TERMS TO BE F.O.B. DESTINATION, PREPAID, UNLESS VENDOR STATES DIFFERENTLY WHEN SUBMITTING THEIR QUOTATION.</p> <p>CANCELLATION: THE DIRECTOR OF PURCHASING RESERVES THE RIGHT TO CANCEL THIS CONTRACT IMMEDIATELY UPON WRITTEN NOTICE TO THE VENDOR IF THE COMMODITIES AND/OR SERVICES SUPPLIED ARE OF AN INFERIOR QUALITY OR DO NOT CONFORM TO THE SPECIFICATIONS OF THE BID AND CONTRACT HEREIN.</p> <p>BANKRUPTCY: IN THE EVENT THE VENDOR/CONTRACTOR FILES FOR BANKRUPTCY PROTECTION, THE STATE MAY DEEM THE CONTRACT NULL AND VOID, AND TERMINATE SUCH CONTRACT WITHOUT FURTHER ORDER.</p>						

RECEIVED
 201 SEP 21 A 9:38
 PURCHASING DIVISION
 STATE OF WV

SEE REVERSE SIDE FOR TERMS AND CONDITIONS			
SIGNATURE	TELEPHONE	DATE	
<i>[Signature]</i>	800-426-8157	September 14, 2011	
TITLE	FEIN	ADDRESS CHANGES TO BE NOTED ABOVE	
VP, Director-Inside Sales	95-4141306		

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED 'VENDOR'



State of West Virginia
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Post Office Box 50130
 Charleston, WV 25305-0130

Request for Quotation

RFQ NUMBER
 LBS12015

PAGE
 2

ADDRESS CORRESPONDENCE TO ATTENTION OF
 ROBERTA WAGNER
 304-558-0067

VENDOR

*506084009 800-426-8157
 QIAGEN INC
 27220 TURNBERRY LANE STE 200
 VALENCIA CA 91355-1005

SHIP TO

HEALTH AND HUMAN RESOURCES
 BPH - LABORATORY SERVICES
 167-ELEVENTH AVENUE
 SOUTH CHARLESTON, WV
 25303 304-558-3530

DATE PRINTED	TERMS OF SALE	SHIP VIA	F.O.B.	FREIGHT TERMS
08/15/2011				

BID OPENING DATE: 09/15/2011 BID OPENING TIME 01:30 PM

LINE	QUANTITY	UOP	CAT. NO.	ITEM NUMBER	UNIT PRICE	AMOUNT
<p>INQUIRIES: WRITTEN QUESTIONS SHALL BE ACCEPTED THROUGH CLOSE OF BUSINESS ON 8/30/2011. QUESTIONS MAY BE SENT VIA USPS, FAX, COURIER OR E-MAIL. IN ORDER TO ASSURE NO VENDOR RECEIVES AN UNFAIR ADVANTAGE, NO SUBSTANTIVE QUESTIONS WILL BE ANSWERED ORALLY. IF POSSIBLE, E-MAIL QUESTIONS ARE PREFERRED. ADDRESS INQUIRIES TO: ROBERTA WAGNER DEPARTMENT OF ADMINISTRATION PURCHASING DIVISION 2019 WASHINGTON STREET, EAST CHARLESTON, WV 25311 FAX: 304-558-4115 E-MAIL: ROBERTA.A.WAGNER@WV.GOV</p> <p>THE MODEL/BRAND/SPECIFICATIONS NAMED HEREIN ESTABLISH THE ACCEPTABLE LEVEL OF QUALITY ONLY AND ARE NOT INTENDED TO REFLECT A PREFERENCE OR FAVOR ANY PARTICULAR BRAND OR VENDOR. VENDORS WHO ARE BIDDING ALTERNATES SHOULD SO STATE AND INCLUDE PERTINENT LITERATURE AND SPECIFICATIONS. FAILURE TO PROVIDE INFORMATION FOR ANY ALTERNATES MAY BE GROUNDS FOR REJECTION OF THE BID. THE STATE RESERVES THE RIGHT TO WAIVE MINOR IRREGULARITIES IN BIDS OR SPECIFICATIONS IN ACCORDANCE WITH SECTION 148-1-4(F) OF THE WEST VIRGINIA LEGISLATIVE RULES AND REGULATIONS.</p> <p>VENDOR PREFERENCE CERTIFICATE</p>						

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE: *Deby Lunder* TELEPHONE: 800-426-8157 DATE: September 14, 2011

TITLE: VP, Director Inside Sales FEIN: 95-4141306 ADDRESS CHANGES TO BE NOTED ABOVE

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED 'VENDOR'



State of West Virginia
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Post Office Box 50130
 Charleston, WV 25305-0130

Request for Quotation

RFQ NUMBER
LBS12015

PAGE
3

ADDRESS CORRESPONDENCE TO ATTENTION OF:
ROBERTA WAGNER 304-558-0067

*506084009 800-426-8157
 QIAGEN INC
 27220 TURNBERRY LANE STE 200
 VALENCIA CA 91355-1005

V
E
N
D
O
R

S
H
I
P
T
O

HEALTH AND HUMAN RESOURCES
 BPH - LABORATORY SERVICES

167-ELEVENTH AVENUE
 SOUTH CHARLESTON, WV
 25303 304-558-3530

DATE PRINTED:	TERMS OF SALE	SHIP VIA	F.O.B.	FREIGHT TERMS
08/15/2011				

BID OPENING DATE: 09/15/2011 BID OPENING TIME 01:30PM

LINE	QUANTITY	UOP	CAT NO	ITEM NUMBER	UNIT PRICE	AMOUNT
<p>THIS TEAM EXHIBIT HAS BEEN REPLACED BY THE ONLINE VERSION WHICH IS AVAILABLE HERE: HTTP://WWW.STATE.WV.US/ADMIN/PURCHASE/VRC/VENPREF.PDF</p> <p style="text-align: center;">NOTICE</p> <p>A SIGNED BID MUST BE SUBMITTED TO:</p> <p style="text-align: center;">DEPARTMENT OF ADMINISTRATION PURCHASING DIVISION BUILDING 15 2019 WASHINGTON STREET, EAST CHARLESTON, WV 25305-0130</p> <p>PLEASE NOTE: A CONVENIENCE COPY WOULD BE APPRECIATED.</p> <p>THE BID SHOULD CONTAIN THIS INFORMATION ON THE FACE OF THE ENVELOPE OR THE BID MAY NOT BE CONSIDERED:</p> <p>SEALED BID</p> <p>BUYER: -----RW/FILE 22-----</p> <p>RFQ. NO.: -----LBS12015-----</p> <p>BID OPENING DATE: -----09/15/2011-----</p> <p>BID OPENING TIME: -----1:30 PM-----</p> <p>PLEASE PROVIDE A FAX NUMBER IN CASE IT IS NECESSARY</p>						

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE <i>Dolly Jumper</i>	TELEPHONE 800-426-8157	DATE September 14, 2011
TITLE VP, Director Inside Sales	FEIN 95-4141306	ADDRESS CHANGES TO BE NOTED ABOVE

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED 'VENDOR'



State of West Virginia
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Post Office Box 50130
 Charleston, WV 25305-0130

Request for Quotation

RFQ NUMBER
 LBS12015

PAGE
 4

ADDRESS CORRESPONDENCE TO ATTENTION OF
 ROBERTA WAGNER
 304-558-0067

VENDOR

*506084009 800-426-8157
 QIAGEN INC
 27220 TURNBERRY LANE STE 200
 VALENCIA CA 91355-1005

SHIP TO

HEALTH AND HUMAN RESOURCES
 BPH - LABORATORY SERVICES
 167-ELEVENTH AVENUE
 SOUTH CHARLESTON, WV
 25303 304-558-3530

DATE PRINTED	TERMS OF SALE	SHIP VIA	F.O.B.	FREIGHT TERMS
08/15/2011				

BID OPENING DATE: 09/15/2011 BID OPENING TIME 01:30PM

LINE	QUANTITY	UOP	CAT. NO.	ITEM NUMBER	UNIT PRICE	AMOUNT
					661-702-3884	
					Oneal Puri, Inside Sales Representative ph: 661-702-3708 email: oneal.puri@qiagen.com	
***** THIS IS THE END OF RFQ LBS12015 ***** TOTAL:						
						Please see QIAGEN quotes #0P091211A, #0P091211B, #0P091411B, each attached hereto and incorporated herein; and RFQ Cost Sheets #1, #2, and #3.

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE *Daley Smith* TELEPHONE 800-426-8157 DATE September 14, 2011
 TITLE VP, Director Inside Sales FEIN 95-4141306 ADDRESS CHANGES TO BE NOTED ABOVE

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED 'VENDOR'

LBS12015

SPECIFICATION AND REQUIREMENTS

Test Equipment Specifications

1. System must be capable of processing 1 - 8 sample purifications from 100ul to 1000ul in 15- 40 minutes.
2. System must be able to track samples and reagents with an integrated bar-code scanner and relabeled Reagent Cartridges and Elution Tubes.
3. System must be able to protect each sample from cross-contamination using synchronized stage movement, integrated HEPA filter, UV decontamination and prefilled and sealed reagents and disposables.
4. System must be able to support magnetic-bead isolation techniques.
5. System must have the following dimensions or less: 540 mm W x 610 mm D x 570 mm H (21.3 in W x 24 in D x 22.4 in H). System must weight 60 kg (132 lbs) or less.
6. System must be capable of producing elution volumes of 50 - 200 ul.
7. System must have a power source of AC 90-240 V, 50/60 Hz.
8. Must be FDA approved.

Computer Equipment Specifications

1. Vendor must supply and integrate any attached personal computer device to the equipment and provide operational configuration and testing.
2. Internal personal computer with windows operating system, operated via color touch screen monitor (6.4 in) and bar-code reader.
3. Instrument must contain preinstalled protocols that can be selected by scanning the bar code on reagent cartridges.
4. System must be capable of saving run documentation, print out with an external printer, or routed via host connectivity.

Installation & Training Requirements

1. Full instrument installation and performance verification must be performed by a Certified Field Service Engineer, must be included at no additional cost and must be completed within 30 days of equipment delivery.
2. One day, on site hands-on training for two people must be performed by a Field Service Engineer at the Office of Laboratory Services, 167 11th Avenue, South Charleston, WV 25303 at no additional cost and must be completed within 30 days of equipment delivery.

Warranty Requirements

1. Must include at least one year equipment warranty to include parts and labor and must be provided at no additional cost.

Service and Support Requirements

1. Must provide full support and service of test equipment and attached computer equipment for the duration of the manufacture warranty and must be provided at no additional cost.

Shipping and Delivery Requirements

1. Shipping terms to be F. O. B. Destination, Prepaid unless vendor states differently when submitting quotation.
2. If shipping costs are incurred they must be included as a separate line item and part of the total cost of the equipment.
3. Must be delivered within 60 days of approved purchase order.
4. Delivery must be inside delivery and must be made Monday through Friday, 8:00 a.m. through 4:00 p.m.

RFQ COST SHEET

Bidders shall provide a cost for the following:

MagNa Pure Compact System, or equal
EZI Advanced XL
EZI Installation

\$ 34,188.75
\$ 17,935.00

Freight/Shipping Charge

\$ 315.98

Total Cost \$ 36,439.73*

* See also QUAGEN quote #OP091411D

The award will be made to the vendor with the lowest overall total cost of the equipment which meets all requested specifications and requirements. Payment will be made in arrears.

Vendor Signature

September 13, 2011
Date


RFQ COST SHEET

Bidders shall provide a cost for the following:

MagNa Pure Compact System, or (equal)	\$ <u>25,000.00</u>
EZI Advanced	<u>\$1,935.00</u>
EZI Installation	
Freight/Shipping Charge	\$ <u>315.98</u>

Total Cost \$ 27,250.98^{*}
 * See also QIAGEN quote #OP091411E

The award will be made to the vendor with the lowest overall total cost of the equipment which meets all requested specifications and requirements. Payment will be made in arrears.

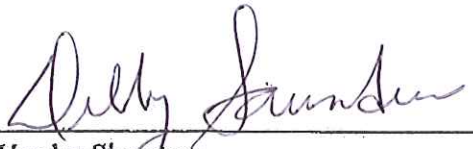
 Vendor Signature

September 14, 2011
 Date

RFQ COST SHEET


Bidders shall provide a cost for the following:

MagNa Pure Compact System, or <u>equal</u>	\$ 85,343.00
QIA Symphony SP	* 4,210.00
QIA Symphony SP Installation	
Freight/Shipping Charge	\$ 508.50

Total Cost \$ 90,061.50*

* See also QIAGEN quote #OP091411h

The award will be made to the vendor with the lowest overall total cost of the equipment which meets all requested specifications and requirements. Payment will be made in arrears.



Vendor Signature

September 14, 2011
Date

ATTACHMENT
P.O.# LBS12015

This agreement constitutes the entire agreement between the parties, and there are no other terms and conditions applicable to the licenses granted hereunder.

Agreed

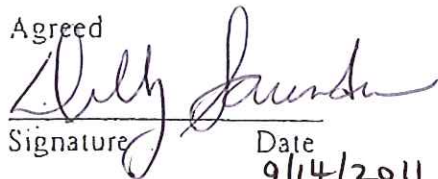
Signature

Date
9/14/2011

VP, Director, Inside Sales
Title

QIAGEN, Inc.
Company Name

Signature Date

Title

Agency/Division

WV-96
Rev. 10/07

AGREEMENT ADDENDUM

In the event of conflict between this addendum and the agreement, this addendum shall control:

1. **DISPUTES** - Any references in the agreement to arbitration or to the jurisdiction of any court are hereby deleted. Disputes arising out of the agreement shall be presented to the West Virginia Court of Claims.
2. **HOLD HARMLESS** - Any clause requiring the Agency to indemnify or hold harmless any party is hereby deleted in its entirety.
3. **GOVERNING LAW** - The agreement shall be governed by the laws of the State of West Virginia. This provision replaces any references to any other State's governing law.
4. **TAXES** - Provisions in the agreement requiring the Agency to pay taxes are deleted. As a State entity, the Agency is exempt from Federal, State, and local taxes and will not pay taxes for any Vendor including individuals, nor will the Agency file any tax returns or reports on behalf of Vendor or any other party.
5. **PAYMENT** - Any references to prepayment are deleted. Payment will be in arrears.
6. **INTEREST** - Should the agreement include a provision for interest on late payments, the Agency agrees to pay the maximum legal rate under West Virginia law. All other references to interest or late charges are deleted.
7. **RECOUPMENT** - Any language in the agreement waiving the Agency's right to set-off, counterclaim, recoupment, or other defense is hereby deleted.
8. **FISCAL YEAR FUNDING** - Service performed under the agreement may be continued in succeeding fiscal years for the term of the agreement, contingent upon funds being appropriated by the Legislature or otherwise being available for this service. In the event funds are not appropriated or otherwise available for this service, the agreement shall terminate without penalty on June 30. After that date, the agreement becomes of no effect and is null and void. However, the Agency agrees to use its best efforts to have the amounts contemplated under the agreement included in its budget. Non-appropriation or non-funding shall not be considered an event of default.
9. **STATUTE OF LIMITATION** - Any clauses limiting the time in which the Agency may bring suit against the Vendor, lessor, individual, or any other party are deleted.
10. **SIMILAR SERVICES** - Any provisions limiting the Agency's right to obtain similar services or equipment in the event of default or non-funding during the term of the agreement are hereby deleted.
11. **ATTORNEY FEES** - The Agency recognizes an obligation to pay attorney's fees or costs only when assessed by a court of competent jurisdiction. Any other provision is invalid and considered null and void.
12. **ASSIGNMENT** - Notwithstanding any clause to the contrary, the Agency reserves the right to assign the agreement to another State of West Virginia agency, board or commission upon thirty (30) days written notice to the Vendor and Vendor shall obtain the written consent of Agency prior to assigning the agreement.
13. **LIMITATION OF LIABILITY** - The Agency, as a State entity, cannot agree to assume the potential liability of a Vendor. Accordingly, any provision limiting the Vendor's liability for direct damages to a certain dollar amount or to the amount of the agreement is hereby deleted. Limitations on special, incidental or consequential damages are acceptable. In addition, any limitation is null and void to the extent that it precludes any action for injury to persons or for damages to personal property.
14. **RIGHT TO TERMINATE** - Agency shall have the right to terminate the agreement upon thirty (30) days written notice to Vendor. Agency agrees to pay Vendor for services rendered or goods received prior to the effective date of termination.
15. **TERMINATION CHARGES** - Any provision requiring the Agency to pay a fixed amount or liquidated damages upon termination of the agreement is hereby deleted. The Agency may only agree to reimburse a Vendor for actual costs incurred or losses sustained during the current fiscal year due to wrongful termination by the Agency prior to the end of any current agreement term.
16. **RENEWAL** - Any reference to automatic renewal is hereby deleted. The agreement may be renewed only upon mutual written agreement of the parties.
17. **INSURANCE** - Any provision requiring the Agency to insure equipment or property of any kind and name the Vendor as beneficiary or as an additional insured is hereby deleted.
18. **RIGHT TO NOTICE** - Any provision for repossession of equipment without notice is hereby deleted. However, the Agency does recognize a right of repossession with notice.
19. **ACCELERATION** - Any reference to acceleration of payments in the event of default or non-funding is hereby deleted.
20. **CONFIDENTIALITY** - Any provision regarding confidentiality of the terms and conditions of the agreement is hereby deleted. State contracts are public records under the West Virginia Freedom of Information Act.
21. **AMENDMENTS** - All amendments, modifications, alterations or changes to the agreement shall be in writing and signed by both parties. No amendment, modification, alteration or change may be made to this addendum without the express written approval of the Purchasing Division and the Attorney General.

ACCEPTED BY:

STATE OF WEST VIRGINIA

Spending Unit: _____

Signed: _____

Title: _____

Date: _____

VENDOR

Company Name: DIAGEN, Inc.

Signed: [Signature]

Title: VP, Director, Inside Sales

Date: September 14, 2011

RFQ No. LBS 12015

STATE OF WEST VIRGINIA
Purchasing Division

PURCHASING AFFIDAVIT

West Virginia Code §5A-3-10a states: No contract or renewal of any contract may be awarded by the state or any of its political subdivisions to any vendor or prospective vendor when the vendor or prospective vendor or a related party to the vendor or prospective vendor is a debtor and the debt owed is an amount greater than one thousand dollars in the aggregate.

DEFINITIONS:

"Debt" means any assessment, premium, penalty, fine, tax or other amount of money owed to the state or any of its political subdivisions because of a judgment, fine, permit violation, license assessment, defaulted workers' compensation premium, penalty or other assessment presently delinquent or due and required to be paid to the state or any of its political subdivisions, including any interest or additional penalties accrued thereon.

"Debtor" means any individual, corporation, partnership, association, limited liability company or any other form or business association owing a debt to the state or any of its political subdivisions. "Political subdivision" means any county commission; municipality; county board of education; any instrumentality established by a county or municipality; any separate corporation or instrumentality established by one or more counties or municipalities, as permitted by law; or any public body charged by law with the performance of a government function or whose jurisdiction is coextensive with one or more counties or municipalities. "Related party" means a party, whether an individual, corporation, partnership, association, limited liability company or any other form or business association or other entity whatsoever, related to any vendor by blood, marriage, ownership or contract through which the party has a relationship of ownership or other interest with the vendor so that the party will actually or by effect receive or control a portion of the benefit, profit or other consideration from performance of a vendor contract with the party receiving an amount that meets or exceeds five percent of the total contract amount.

EXCEPTION: The prohibition of this section does not apply where a vendor has contested any tax administered pursuant to chapter eleven of this code, workers' compensation premium, permit fee or environmental fee or assessment and the matter has not become final or where the vendor has entered into a payment plan or agreement and the vendor is not in default of any of the provisions of such plan or agreement.

Under penalty of law for false swearing (*West Virginia Code* §61-5-3), it is hereby certified that the vendor affirms and acknowledges the information in this affidavit and is in compliance with the requirements as stated.

WITNESS THE FOLLOWING SIGNATURE

Vendor's Name: BIAGEN, Inc.

Authorized Signature: *[Signature]* Date: September 14, 2011

State of Maryland

County of Frederick, to-wit:

Taken, subscribed, and sworn to before me this 14th day of September, 2011.

My Commission expires May 16, 2014.

AFFIX SEAL HERE

NOTARY PUBLIC *[Signature]*

N/A

State of West Virginia

VENDOR PREFERENCE CERTIFICATE

Certification and application* is hereby made for Preference in accordance with West Virginia Code, §5A-3-37. (Does not apply to construction contracts). West Virginia Code, §5A-3-37, provides an opportunity for qualifying vendors to request (at the time of bid) preference for their residency status. Such preference is an evaluation method only and will be applied only to the cost bid in accordance with the West Virginia Code. This certificate for application is to be used to request such preference. The Purchasing Division will make the determination of the Resident Vendor Preference, if applicable.

- 1. Application is made for 2.5% resident vendor preference for the reason checked: Bidder is an individual resident vendor and has resided continuously in West Virginia for four (4) years immediately preceding the date of this certification; or, Bidder is a partnership, association or corporation resident vendor and has maintained its headquarters or principal place of business continuously in West Virginia for four (4) years immediately preceding the date of this certification; or 80% of the ownership interest of Bidder is held by another individual, partnership, association or corporation resident vendor who has maintained its headquarters or principal place of business continuously in West Virginia for four (4) years immediately preceding the date of this certification; or, Bidder is a nonresident vendor which has an affiliate or subsidiary which employs a minimum of one hundred state residents and which has maintained its headquarters or principal place of business within West Virginia continuously for the four (4) years immediately preceding the date of this certification; or,
2. Application is made for 2.5% resident vendor preference for the reason checked: Bidder is a resident vendor who certifies that, during the life of the contract, on average at least 75% of the employees working on the project being bid are residents of West Virginia who have resided in the state continuously for the two years immediately preceding submission of this bid; or,
3. Application is made for 2.5% resident vendor preference for the reason checked: Bidder is a nonresident vendor employing a minimum of one hundred state residents or is a nonresident vendor with an affiliate or subsidiary which maintains its headquarters or principal place of business within West Virginia employing a minimum of one hundred state residents who certifies that, during the life of the contract, on average at least 75% of the employees or Bidder's affiliate's or subsidiary's employees are residents of West Virginia who have resided in the state continuously for the two years immediately preceding submission of this bid; or,
4. Application is made for 5% resident vendor preference for the reason checked: Bidder meets either the requirement of both subdivisions (1) and (2) or subdivision (1) and (3) as stated above; or,
5. Application is made for 3.5% resident vendor preference who is a veteran for the reason checked: Bidder is an individual resident vendor who is a veteran of the United States armed forces, the reserves or the National Guard and has resided in West Virginia continuously for the four years immediately preceding the date on which the bid is submitted; or,
6. Application is made for 3.5% resident vendor preference who is a veteran for the reason checked: Bidder is a resident vendor who is a veteran of the United States armed forces, the reserves or the National Guard, if, for purposes of producing or distributing the commodities or completing the project which is the subject of the vendor's bid and continuously over the entire term of the project, on average at least seventy-five percent of the vendor's employees are residents of West Virginia who have resided in the state continuously for the two immediately preceding years.

Bidder understands if the Secretary of Revenue determines that a Bidder receiving preference has failed to continue to meet the requirements for such preference, the Secretary may order the Director of Purchasing to: (a) reject the bid; or (b) assess a penalty against such Bidder in an amount not to exceed 5% of the bid amount and that such penalty will be paid to the contracting agency or deducted from any unpaid balance on the contract or purchase order.

By submission of this certificate, Bidder agrees to disclose any reasonably requested information to the Purchasing Division and authorizes the Department of Revenue to disclose to the Director of Purchasing appropriate information verifying that Bidder has paid the required business taxes, provided that such information does not contain the amounts of taxes paid nor any other information deemed by the Tax Commissioner to be confidential.

Under penalty of law for false swearing (West Virginia Code, §61-5-3), Bidder hereby certifies that this certificate is true and accurate in all respects; and that if a contract is issued to Bidder and if anything contained within this certificate changes during the term of the contract, Bidder will notify the Purchasing Division in writing immediately.

Bidder: _____ Signed: _____

Date: _____ Title: _____

*Check any combination of preference consideration(s) indicated above, which you are entitled to receive.



September 14, 2011

Roberta Wagner
Laboratory Services
Department of Administration
Purchasing Division
2019 Washington Street East
Charleston, WV 25305 - 0130

RE: QIAGEN Agreement # OP091411D

Dear Roberta Wagner,

Thank you for your interest in QIAGEN solutions. I have enclosed the quotation you requested. Please note that the terms and conditions, including shipping, are located on the first page of the attached quotation. When placing an order, please reference the Agreement Number shown above and at the top of the quotation to ensure accurate pricing and shipping.

Thank you for considering QIAGEN products. If you have any questions, please call me at 661-702 3708 ext. 23708.

Sincerely,

Oneal Puri
Inside Sales Representative

QIAGEN - Sample & Assay Technologies

QUOTATION

QIAGEN Agreement # OP091411D

September 14, 2011



Roberta Wagner
 Laboratory Services
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Charleston, WV 25305 - 0130
 Phone: +1 (304) 558-3530

Delivery: 30-75 days ARO	F.O.B. Instrument: Shipping Point - Freight Prepaid and Added	Prices Valid For: 60 days	Terms: Net 30 Days Upon Invoicing
<p>QIAGEN's Response to RFQ#LBS12015, Robotic workstation for automated purification of nucleic acids from up to 14 samples using EZ1 kits. 1-year warranty on parts and labor included. Installation, performance verification and one day, on-site hands-on training to be performed within 30 days of equipment delivery by a QIAGEN certified Service Engineer is also included.</p> <p>QIAGEN's total response to RFQ# LBS12015 = \$36,439.73</p>			

Item	Catalog #	Description	Unit Price	Qty	Extended Price
1	9001492	EZ1 Advanced XL	34,188.75	1	34,188.75
2	9237713	EZ1, Installation The Installation, BR EZ1 facilitates the quick implementation of the BioRobot EZ1 or EZ1 Advanced into the lab routine by minimizing the instrument start-up phase. It covers the hardware and software installation of the BioRobot EZ1 or EZ1 Advanced instrument and provides the user with an introductory training on operation and user maintenance. The installation includes labor and travel costs. The performance of the installation process is documented on a GMP/GLP-compliant Field Service document.	1,935.00	1	1,935.00
3	9018694	EZ1 Adv. XL DNA Bacteria Card	Included	1	Included
4	9018708	EZ1 Adv. XL Virus Card v2.0	Included	1	Included
5	1002137	Freight charges	315.98	1	315.98

Please note the following:

- System installation is not included unless specified above. If installation is purchased, QIAGEN will install the protocol, test the protocol, and backup the system software and protocol.
- Instrument shipped upon availability. Actual delivery times may vary.
- Payment due 30 days upon invoicing. QIAGEN will provide installation and introductory training upon delivery. If the Customer delays installation and/or introductory training for more than four weeks after delivery, payment for the instrument is due by the Customer.
- This proposal is made contingent upon the acceptance by Customer without changes or modification of the provisions of this proposal including all insertions on the face hereof and of the QIAGEN terms and conditions of sales provided.

***Quoted Price: \$ 36,439.73**

*Shipping not included in quoted price

This Quote shall be governed by the QIAGEN Standard Terms and Conditions available at <http://www.qiagen.com/SalesTermsUS>

QUOTATION

Oneal Puri
Inside Sales Representative
661-702 3708 ext. 23708

QIAGEN - Sample & Assay Technologies

To place order by phone: 800-426-8157
On-line: www.qiagen.com
Fax: 661-702-3884
email: instrumentorders@qiagen.com
Mail: QIAGEN Inc.
27220 Turnberry Lane, Suite 200
Valencia, CA 91355-1005



September 14, 2011

Roberta Wagner
Laboratory Services
Department of Administration
Purchasing Division
2019 Washington Street East
Charleston, WV 25305 - 0130

RE: QIAGEN Agreement # OP091411E

Dear Roberta Wagner,

Thank you for your interest in QIAGEN solutions. I have enclosed the quotation you requested. Please note that the terms and conditions, including shipping, are located on the first page of the attached quotation. When placing an order, please reference the Agreement Number shown above and at the top of the quotation to ensure accurate pricing and shipping.

Thank you for considering QIAGEN products. If you have any questions, please call me at 661-702 3708 ext. 23708.

Sincerely,

Oneal Puri
Inside Sales Representative

QIAGEN - Sample & Assay Technologies

QUOTATION

QIAGEN Agreement # OP091411E

September 14, 2011



Roberta Wagner
 Laboratory Services
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Charleston, WV 25305 - 0130
 Phone: +1 (304) 558-3530

Delivery: 30-75 days ARO	F.O.B. Instrument: Shipping Point - Freight Prepaid and Added	Prices Valid For: 60 days	Terms: Net 30 Days Upon Invoicing
<p>QIAGEN's Response to RFQ#LBS12015, Robotic workstation for automated purification of nucleic acids using EZ1 kits. 1-year warranty on parts and labor included. Installation, performance verification and one day, on-site hands-on training to be performed within 30 days of equipment delivery by a QIAGEN certified Service Engineer is also included.</p> <p>QIAGEN's total response to RFQ# LBS12015 = \$27,250.98</p>			

Item	Catalog #	Description	Unit Price	Qty	Extended Price
1	9001410	EZ1 Advanced	25,000.00	1	25,000.00
2	9237713	EZ1, Installation The Installation, BR EZ1 facilitates the quick implementation of the BioRobot EZ1 or EZ1 Advanced into the lab routine by minimizing the instrument start-up phase. It covers the hardware and software installation of the BioRobot EZ1 or EZ1 Advanced instrument and provides the user with an introductory training on operation and user maintenance. The installation includes labor and travel costs. The performance of the installation process is documented on a GMP/GLP-compliant Field Service document.	1,935.00	1	1,935.00
3	9018301	EZ1 Advanced DNA Bacteria Card	Included	1	Included
4	9018303	EZ1 Advanced Virus Card v2.0	Included	1	Included
5	1002137	Freight charges	315.98	1	315.98

Please note the following:

1. System installation is not included unless specified above. If installation is purchased, QIAGEN will install the protocol, test the protocol, and backup the system software and protocol.
2. Instrument shipped upon availability. Actual delivery times may vary.
3. Payment due 30 days upon invoicing. QIAGEN will provide installation and introductory training upon delivery. If the Customer delays installation and/or introductory training for more than four weeks after delivery, payment for the instrument is due by the Customer.
4. This proposal is made contingent upon the acceptance by Customer without changes or modification of the provisions of this proposal including all insertions on the face hereof and of the QIAGEN terms and conditions of sales provided.

***Quoted Price: \$ 27,250.98**

*Shipping not included in quoted price

This Quote shall be governed by the QIAGEN Standard Terms and Conditions available at <http://www.qiagen.com/SalesTermsUS>

QUOTATION

Oneal Puri
Inside Sales Representative
661-702 3708 ext. 23708

QIAGEN Sample & Assay Technologies

To place order by phone: 800-426-8157
On-line: www.qiagen.com
Fax: 661-702-3884
email: instrumentorders@qiagen.com
Mail: QIAGEN Inc.
27220 Turnberry Lane, Suite 200
Valencia, CA 91355-1005



September 14, 2011

Roberta Wagner
Laboratory Services
Department of Administration
Purchasing Division
2019 Washington Street East
Charleston, WV 25305 - 0130

RE: QIAGEN Agreement # OP091411h

Dear Roberta Wagner,

Thank you for your interest in QIAGEN solutions. I have enclosed the quotation you requested. Please note that the terms and conditions, including shipping, are located on the first page of the attached quotation. When placing an order, please reference the Agreement Number shown above and at the top of the quotation to ensure accurate pricing and shipping.

Thank you for considering QIAGEN products. If you have any questions, please call me at 661-702 3708 ext. 23708.

Sincerely,

Oneal Puri
Inside Sales Representative

QIAGEN - Sample & Assay Technologies

QUOTATION



QIAGEN Agreement # OP091411h

September 14, 2011

Roberta Wagner
 Laboratory Services
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Charleston, WV 25305 - 0130
 Phone: +1 (304) 558-3530

Delivery: 30-75 days ARO	F.O.B. Instrument: Shipping Point - Freight Prepaid and Added	Prices Valid For: 60 days	Terms: Net 30 Days Upon Invoicing
<p>QIAGEN's Response to RFQ#LBS12015</p> <p>QIASymphony sample prep module, 1-year warranty on parts and labor.</p> <p>For fully integrated automation of complete workflows, from sample preparation to assay setup Innovative, easy-to-use modular system with built-in touchscreen Purification of DNA, RNA, and protein from a wide range of sample types Automatic transfer of eluates to the QIASymphony AS for assay setup Continuous sample loading with bar code reading for full sample tracking Import of sample lists and export of sample sheets</p> <p>QIAGEN's total response to RFQ# LBS12015 = \$90,061.50</p>			

Item	Catalog #	Description	Unit Price	Qty	Extended Price
1	9001297	QIASymphony SP	85,343.00	1	85,343.00
2	9240372	QIASymphony SP, Installation The Installation, QIASymphony SP facilitates the quick implementation of the QIASymphony into the lab routine by minimizing the instrument start-up phase. It covers the hardware and software installation of the QIASymphony instrument and provides the user with an introductory training. The installation includes or labor and travel costs. The performance of the installation process is documented on a GMP/GLP-compliant Field Service document.	4,210.00	1	4,210.00
3	1002137	Freight charges	508.50	1	508.50

Please note the following:

- System installation is not included unless specified above. If installation is purchased, QIAGEN will install the protocol, test the protocol, and backup the system software and protocol.
- Instrument shipped upon availability. Actual delivery times may vary.
- Payment due 30 days upon invoicing. QIAGEN will provide installation and introductory training upon delivery. If the Customer delays installation and/or introductory training for more than four weeks after delivery, payment for the instrument is due by the Customer.
- This proposal is made contingent upon the acceptance by Customer without changes or modification of the provisions of this proposal including all insertions on the face hereof and of the QIAGEN terms and conditions of sales provided.

***Quoted Price: \$ 90,061.50**

*Shipping not included in quoted price

This Quote shall be governed by the QIAGEN Standard Terms and Conditions available at <http://www.qiagen.com/SalesTermsUS>

QUOTATION

Oneal Puri
Inside Sales Representative
661-702 3708 ext. 23708

QIAGEN - Sample & Assay Technologies

To place order by phone: 800-426-8157
On-line: www.qiagen.com
Fax: 661-702-3884
email: instrumentorders@qiagen.com
Mail: QIAGEN Inc.
27220 Turnberry Lane, Suite 200
Valencia, CA 91355-1005

EZ1[®] Advanced — pure convenience

New



Sample & Assay Technologies

Improved walkaway automation for results you can depend on

The EZ1 Advanced builds on and extends the functionality of the well-established and highly successful BioRobot® EZ1. The improved workstation provides the convenience and reliability laboratories worldwide have come to rely on, together with a new design and new features — ensuring effortless data management and improved safety.

The new EZ1 Advanced enables nucleic acid purification from a wide range of samples for genetic identity testing, forensics, biomedical research, and gene expression analysis. The combination of easy-to-use workstation, with error-free protocol selection and worktable setup, and prefilled, sealed reagent cartridges makes nucleic acid purification easy.

The EZ1 Advanced workstation delivers:

- Effortless data management with full traceability
- UV decontamination for a safe user environment
- Flexible throughput by connecting multiple units
- High-quality genomic DNA and RNA from a range of sample materials
- Viral nucleic acids from serum, plasma, and CSF

Proven performance is guaranteed

The new instrument uses proven EZ1 Kits with improved protocols on EZ1 Advanced Cards. Performance of the EZ1 Advanced is equivalent to or better than the BioRobot EZ1 (Figure 1).

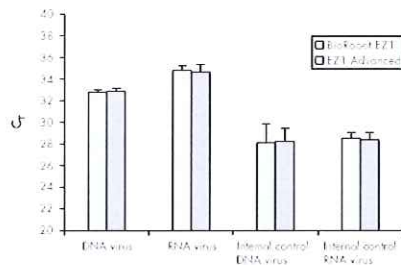


Figure 1. Equivalent performance to the highly successful BioRobot EZ1. Human EDTA plasma was spiked with a DNA and RNA virus. Viral nucleic acids were purified in parallel on the BioRobot EZ1 and on the new EZ1 Advanced using the EZ1 Virus Mini Kit v2.0 and the EZ1 Virus Card v2.0 or EZ1 Advanced Virus Card v2.0. Nucleic acids were detected with real-time duplex PCR and RT-PCR and analyzed on an ABI PRISM® 7900HT Sequence Detection System.

Easy, safe, and reliable

Safety and reliability

The improved design means that the EZ1 Advanced can be placed in a laminar flow hood, if required, providing increased user safety. At the end of each protocol, an intelligent-design UV lamp decontaminates the inner surface of the workstation, which helps to eliminate sample carryover from run-to-run.

Standardization and traceability


The EZ1 Advanced sets new standards in data management. Bar code reading enables complete tracking of samples and reagents throughout the entire purification process. The automatically generated run report contains all instrument information, including maintenance procedures and decontamination data.

Flexibility and ease of use

The EZ1 Advanced offers a wide range of protocols for purification of DNA, RNA, or viral nucleic acids from 1–6 samples per run. Up to 4 EZ1 Advanced instruments can be connected to an external computer (supplied by QIAGEN), expanding your throughput to 1–24 samples per run.

Proven technology with improved performance

Proven magnetic-particle technology ensures high-performance results. With new features that provide increased process safety, the EZ1 Advanced makes your purification procedures easy, safe, and reliable.

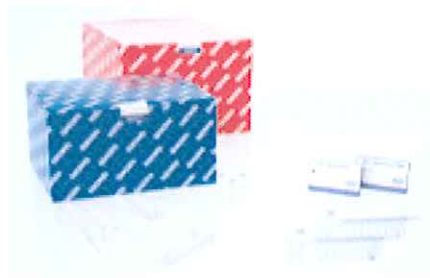

Visit www.qiagen.com/goto/EZ1Advanced to discover just how easy, safe, and reliable walkaway automation can be!



Ordering Information

Product	Contents	Cat. no.
EZ1 Advanced	Robotic workstation for automated purification of nucleic acids using EZ1 Kits, 1-year warranty on parts and labor*	9001410
EZ1 Advanced DSP†	Robotic workstation for automated purification of nucleic acids using EZ1 DSP Kits, 1-year warranty on parts and labor‡	9001411

IQ/OQ Services

IQ/OQ Services	Validation support service for EZ1 Advanced and BioRobot EZ1 workstations. Validation support provides IQ/OQ documentation and performance of the qualification protocols with costs for labor and travel covered	9240826
----------------	---	---------

* Warranty PLUS 2 (cat. no. 9237720) recommended: 3-year warranty, 1 preventive maintenance visit per year, 48-hour priority response, all labor, travel, and repair parts. † Not available in all countries, please inquire. For information about CE-IVD marked purification kits, visit www.qiagen.com. ‡ Warranty PLUS 2 (cat. no. 9240811) recommended: 3-year warranty, 1 preventive maintenance visit per year, 48-hour priority response, all labor, travel, and repair parts.

The EZ1 Advanced Workstation and EZ1 Advanced Cards are intended for research applications. No claim or representation is intended for their use to provide information for the diagnosis, prevention, or treatment of a disease. EZ1 Kits are intended for general laboratory use. No claim or representation is intended to provide information for the diagnosis, prevention, or treatment of a disease.

The EZ1 Advanced DSP System is intended for in-vitro diagnostic use in Europe.

Trademarks: QIAGEN®, BioRobot®, EZ1® (QIAGEN Group); AEF FRISM® (Apple Corporation or its subsidiaries). © 2008 QIAGEN, all rights reserved.
1050552 - 01/2008

www.qiagen.com

Australia # 1-800-243-800
Austria # 0800/281010
Belgium # 0800-79612
Canada # 800-572-9613
China # 021-51345678
Denmark # 80-885945

Finland # 0800-914416
France # 01-60-920-930
Germany # 02103-29-12000
Hong Kong # 800-933-965
Ireland # 1800-555-049
Italy # 800-787980
Japan # 03-5547-0811
Korea (South) # 1544-7145

Luxembourg # 8002-2076
The Netherlands # 0800-0229592
Norway # 800-18859
Singapore # 65-67775366
Sweden # 020-790282
Switzerland # 055-254-22-11
UK # 01293-422-911
USA # 800-426-8157



Sample & Assay Technologies

QIASymphony[®] SP — Pure Performance




Sample & Assay Technologies




Fully automated sample and assay technologies

By combining performance-leading QIAGEN[†] magnetic-particle chemistry with a broad application range for RNA, DNA, and protein purification, the QIASymphony SP sets a new milestone in automated sample technologies. Cutting-edge technology, innovative functions, and optimized protocols, plus processing of large sample volumes^{*} give you high-performance results you can trust. The QIASymphony SP is the first module in the new QIASymphony series of automated systems, which provides automation of your complete workflow — from sample to assay.[†]

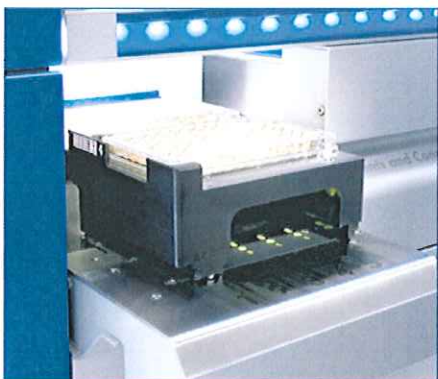

Loading of samples in plate format.

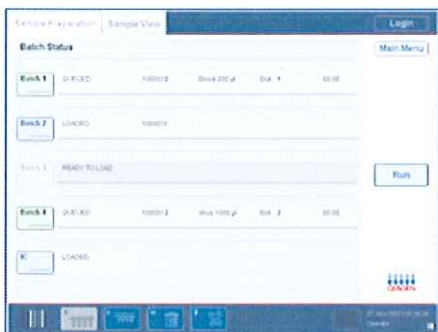

Intuitive, easy-to-use software.

The QIASymphony SP enables your success in:

- Molecular diagnostics research and biomedical research
- Human identity testing, veterinary applications, and biosecurity research
- Life science applications, such as genomics and proteomics research

The QIASymphony SP takes ease of use to a new level

The QIASymphony SP is ready-to-run and requires only minimal installation, enabling fast startup in your laboratory. The QIASymphony SP is operated via an integrated touchscreen, and up to 96 samples, reagents, and plasticware are loaded into drawers, providing increased ease of use and user safety. Innovative reagent cartridges enable processing of a wide range of starting materials with just a few kits. Bar code reading throughout the entire purification procedure enables full process documentation.

The QIASymphony SP delivers pure performance:

- Purify DNA, RNA, or proteins from up to 96 samples
- Proven, performance-leading magnetic-particle chemistries
- Built-in flexibility for laboratory workflow integration
- Cutting-edge process control for safe operation
- Modular system for automation of complete workflows[†]

^{*} 1 ml sample volumes can be processed when running certain applications (e.g., purification of viral nucleic acids or genomic DNA from blood).

[†] An automated assay setup system is currently under development; for more information, please inquire.

Unrivaled application range


QIASymphony Kits — backed by QIAGEN Quality™— increase laboratory efficiency since just a few kits in combination with optimized protocols cover an extensive range of starting materials and applications (Table 1). Sample volumes of up to 1000 µl and up to 50 mg of tissue or 10⁷ cells can be processed, providing increased nucleic acid yields for gene expression and genomics applications and higher sensitivity in virology and microbiology applications. The QIASymphony SP delivers pure performance in virus and bacteria applications and makes no compromise when purifying DNA from blood, RNA from tissues and cells, or proteins from *E. coli* or eukaryotic cells. For up-to-date information about QIASymphony applications, visit www.qiagen.com/goto/QIASymphony.

Innovative kit concept for ease-of-use and improved efficiency

QIASymphony Kits are exceptionally easy to use. Innovative, ready-to-run reagent cartridges are prefilled with all reagents required for the purification procedure, including accessory enzymes. Worktable setup is rapid, which saves your valuable time. Simply place up to 2 reagent cartridges in the QIASymphony drawer. The reagent cartridges can be either from the same kit or from different kits, enabling different purification procedures to be performed within the same run of 96 samples. Reagent cartridges are automatically opened by the instrument and reagent volumes only for the selected number of samples are used, giving you complete cost control.

QIASymphony reagent cartridges are safe and fully trackable

QIASymphony reagent cartridges enable increased process safety and eliminate tedious manual documentation. Prefilled, sealed reagent cartridges eliminate pouring of reagents. Reagent cartridges, including accessory enzymes, are labeled with 2D bar codes, enabling automatic recognition by the QIASymphony SP and tracking of individual reagents throughout the entire purification procedure. Used reagent lots for each batch of samples are documented in the final result file.

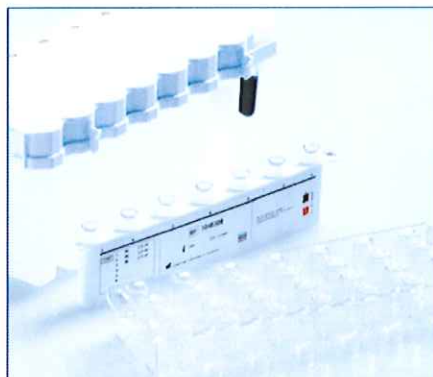


Prefilled, sealed reagent cartridges are bar code labeled and ready to use.



Automated heated lysis and purification from sample volumes of up to 1 ml.




Two reagent cartridges can be loaded per run.

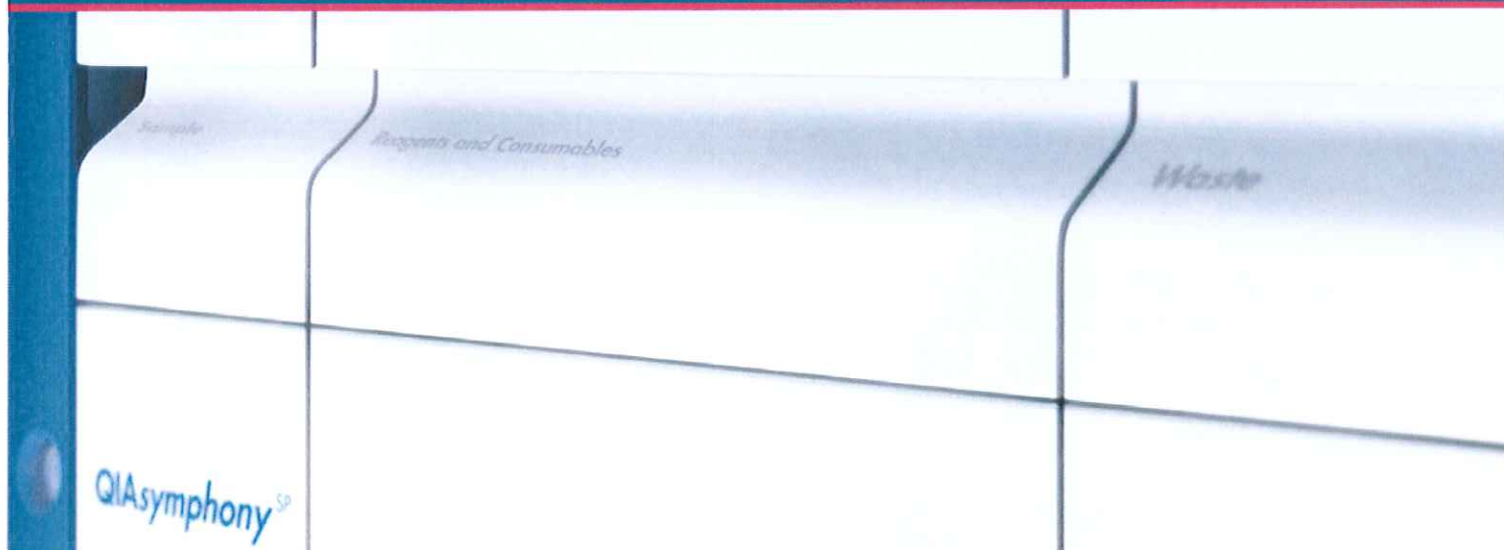

Separate compartments for convenient and easy handling

The QIASymphony SP makes automated sample preparation easier and more convenient than ever. Instrument setup for a run of 96 samples can be performed in just a few minutes, enabling efficient use of your time. Samples, reagents and consumables, and eluates are separated in different drawers. Simply load samples, reagent cartridges, and preracked consumables into the appropriate drawers before the protocol starts. Select your protocol and remove purified nucleic acids or proteins from the eluate drawer after processing.

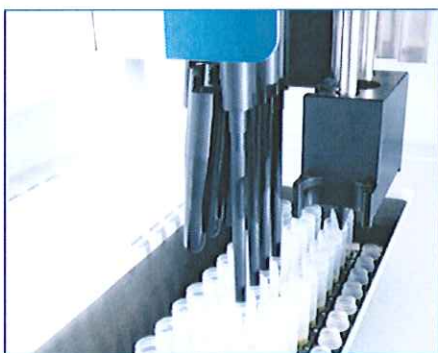

Automated sample transfer from primary tubes.

Flexibility for seamless workflow integration

The sample input drawer accommodates a wide range of sample input formats to suit your workflow and sample preparation requirements. By using the appropriate tube or plate rack, you can load a variety of tube and plate types, including bar code labeled primary tubes from 10–16.9 mm or 96-well plates or blocks. Tubes in 4 racks of 24 samples or up to four 96-well plates or blocks can be placed in the sample input drawer. Bar codes are automatically read as the sample carrier slides into the instrument, enabling sample tracking throughout the purification process.



Automated bar code reading of sample tubes.

In-process sample loading* and prioritization of urgent samples

The high-performance specifications of the QIASymphony SP include in-process sample loading. This advanced feature enables you to load additional sample racks during an ongoing protocol run, making sample preparation even more time efficient and convenient. Simply select the protocol and queue samples for processing after the current batch. Furthermore, you can prioritize the processing order of queued batches to enable preparation of urgent samples.

* For availability of this feature, please inquire.

Choice of elution formats

Purified nucleic acids or proteins are eluted into tubes or plates. Four different elution positions are available and eluates can also be cooled. Eluates can be removed from the output drawer at the end of the protocol run or after a batch of 24 samples has been processed — giving you added flexibility.

Intuitive system


The QIAAsymphony SP is an intuitive, easy-to-use system. An integrated touch-screen enables easy protocol selection, and parameters such as elution volume or type of labware can be selected to suit the requirements of your downstream applications. The QIAAsymphony SP is preinstalled with optimized protocols for purification of nucleic acids or proteins from a wide range of starting materials (Table 1).

Advanced process safety

With its innovative design, the QIAAsymphony SP delivers exceptional process safety and standardized sample preparation. Safety features such as enhanced liquid-level detection and clot detection contribute to the robustness of the purification procedure. In addition, tip guards help to minimize the risk of cross-contamination and an integrated UV light enables decontamination of the worktable. Prefilled reagent cartridges and automatic recognition of reagent cartridges combined with a detailed inventory scan helps to ensure that the system has everything it needs for the protocol. Bar code reading of reagents as well as samples and eluates enables full tracking throughout the entire purification procedure — from sample to eluate.



Choice of elution formats, including cooling.

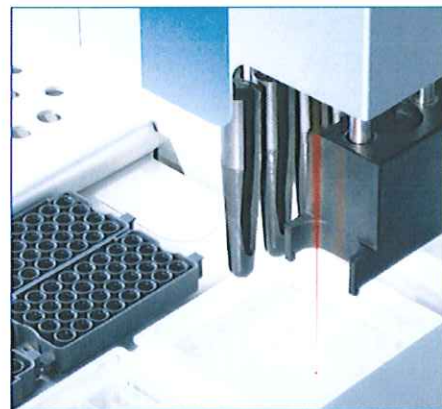

Detailed inventory check helps to eliminate human error.

Table 1. Flexible processing of a wide range of samples


QIAAsymphony Kit	Starting material and amount
QIAAsymphony Virus/Bacteria Kits	Purification of viral nucleic acids from up to 1000 µl plasma, serum, or CSF Purification of viral nucleic acids and bacterial DNA from 200 µl respiratory samples, up to 800 µl urine or transport media, or air-dried swabs
QIAAsymphony DNA Kits	Purification of DNA from up to 1000 µl human whole blood, 400 µl buffy coat, 50 mg tissue, or 1×10^7 cells
QIAAsymphony DNA Investigator Kit	Purification of reference and casework samples for human identity testing and forensics
QIAAsymphony RNA Kit	Purification of total RNA from up to 50 mg tissue or 1×10^7 cells
QIAAsymphony PAXgene™ Blood RNA Kit*	Purification of cellular RNA from 2.5 ml human whole blood collected in PAXgene Blood RNA Tubes
QIAAsymphony PCR Purification Kit	Purification of PCR products from up to 100 µl amplification reactions
QIAAsymphony Ni-NTA Native Kit	Purification of 6xHis-tagged proteins from up to 5 ml <i>E. coli</i> or up to 2.5×10^7 eukaryotic cells
QIAAsymphony Ni-NTA Denaturing Kit	Purification of 6xHis-tagged proteins from up to 5 ml <i>E. coli</i> or up to 2.5×10^7 eukaryotic cells

* Up to 48 samples can be processed per run.



QIAGEN Device Management enhances process efficiency

At QIAGEN, one of our key goals is to help you achieve outstanding success in your laboratory work. To meet your demands, we provide state-of-the-art service and support for your automated applications.

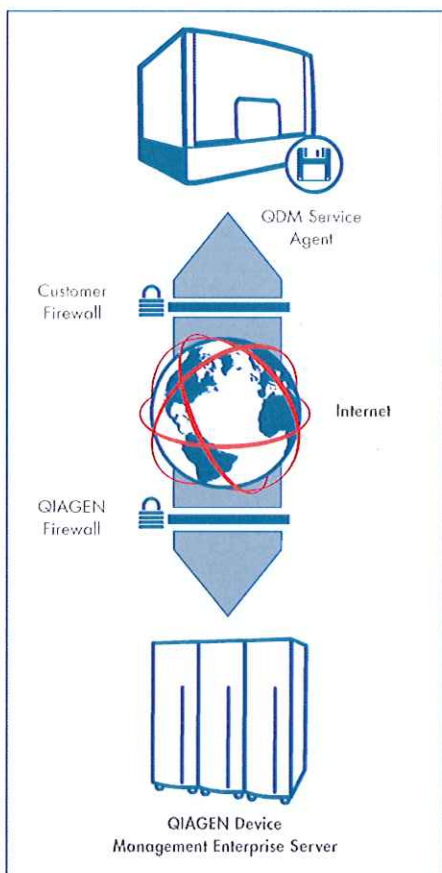

Through novel service capabilities, we enable increased availability and productivity of your QIASymphony SP. On request, QIAGEN Device Management can send instrument data from your QIASymphony SP through an encrypted, secure link to our in-house server, enabling faster service response times and maximum instrument uptime. You benefit from optimal instrument performance and early and accurate diagnosis of problems.

Comprehensive service and support

QIAGEN Instrument Service provides flexible service support agreements tailored to your needs. We also provide Warranty PLUS extended warranties, giving you complete cost control and enhanced coverage through priority response times.

Table 2. Specifications of the QIASymphony SP

Dimensions	Width: 130 cm [51.2 in.]
	Depth: 75 cm [29.5 in.] drawer closed 125 cm [49.2 in.] drawer open
	Height: 103 cm [40.6 in.] door closed 163 cm [64.2 in.] door open
Weight	175 kg (385.8 lb.) 220 kg (485 lb.) with packaging
Electrical requirements	100–240 V AC, 50–60 Hz \pm 10%, 800 VA
Sample throughput	1–96 samples per run
Sample input volume	Up to 1000 μ l
Warranty	1-year warranty on parts and labor

Visit www.qiagen.com/goto/QIASymphony to discover more about the QIASymphony SP!

Ordering Information

Product*	Contents	Cat. no.
QIASymphony SP	QIASymphony sample prep module, 1-year warranty on parts and labor [†]	9001297
QIASymphony Virus/Bacteria Mini Kit (192) [‡]	For up to 192 preps of 200 µl each: Includes 2 reagent cartridges and enzyme racks and accessories	931036
QIASymphony Virus/Bacteria Midi Kit (96) [‡]	For up to 96 preps of 1000 µl each: Includes 2 reagent cartridges and enzyme racks and accessories	931055
QIASymphony DNA Mini Kit (192) [‡]	For 192 preps of 200 µl each: Includes 2 reagent cartridges and enzyme racks and accessories	931236
QIASymphony DNA Midi Kit (96) [‡]	For 96 preps of 1000 µl each: Includes 2 reagent cartridges and enzyme racks and accessories	931255
QIASymphony DNA Investigator Kit (192) [‡]	For 192 preps from casework and reference samples: Includes 2 reagent cartridges and enzyme racks and accessories	931436
QIASymphony RNA Kit (192)	For 192 preps: Includes 2 reagent cartridges and enzyme racks and accessories	931636
QIASymphony PAXgene Blood RNA Kit (96)	For 96 preps: Includes 2 reagent cartridges and enzyme racks and accessories	762535
QIASymphony PCR Purification Kit (192)	For 192 preps: Includes 2 reagent cartridges and enzyme racks and accessories	932036
QIASymphony Ni-NTA Native Kit (384)	For 384 micro-scale preps or 48 medium-scale preps: Includes 2 reagent cartridges and enzyme racks and accessories	932636
QIASymphony Ni-NTA Denaturing Kit (384)	For 384 micro-scale preps or 48 medium-scale preps: Includes 2 reagent cartridges and enzyme racks and accessories	932836
Sample Prep Cartridges, 8-well (336)	8-well Sample Prep Cartridges for use with the QIASymphony SP	997002
8-Rod Covers (144)	8-Rod Covers for use with the QIASymphony SP	997004
Filter-Tips, 200 µl (1024)	Sterile, Disposable Filter-Tips, racked; (8 x 128)	990332
Filter-Tips, 1500 µl (1024)	Sterile, Disposable Filter-Tips, racked; (8 x 128)	997024

* Not all features and products described will be available in Q2 2008, please inquire.

[†] A comprehensive range of service agreements is available; please inquire.

[‡] An additional buffer may be required for some sample types; please inquire.

The QIASymphony SP is intended to be used only in combination with QIASymphony Kits for applications described in the respective QIASymphony Kit handbooks. QIASymphony DNA Kits and QIASymphony Virus/Bacteria Kits are intended for general laboratory use. No claim or representation is intended to provide information for the diagnosis, prevention, or treatment of a disease. The QIASymphony PAXgene Blood RNA Kit and QIASymphony RNA Kit: For Research Use Only. Not for use in diagnostics procedures. No claim or representation is intended to provide information for the diagnosis, prevention, or treatment of a disease.

www.qiagen.com

Australia • Orders 03 9840 9800 • Fax 03 9840 9888 • Technical 1 800 243 066

Austria • Orders 0800/28-10-10 • Fax 0800/28-10-19 • Technical 0800/28-10-11

Belgium • Orders 0800-79612 • Fax 0800-79611 • Technical 0800-79556

Canada • Orders 800 572 9613 • Fax 800 713 5951 • Technical 800-DNA-PREP (800-362 7737)

China • Orders 021-51345678 • Fax 021-51342500 • Technical 021-51345678

Denmark • Orders 80-885945 • Fax 80-885944 • Technical 80-885942

Finland • Orders 0800 914416 • Fax 0800 914415 • Technical 0800 914413

France • Orders 01-60-920-920 • Fax 01-60-920-925 • Technical 01-60-920-930

Germany • Orders 02103-29-12000 • Fax 02103-29-22000 • Technical 02103-29-12400

Hong Kong • Orders 800 933 965 • Fax 800 930 439 • Technical 800 930 425

Ireland • Orders 1800 555 049 • Fax 1800 555 048 • Technical 1800 555 061

Italy • Orders 02-33430411 • Fax 02-33430426 • Technical 800 787980

Japan • Orders: 03-5547-0911 • Fax 03-5547-0818 • Technical 03-5547-0811

Korea (South) • Orders 1544 7145 • Fax 1544 7146 • Technical 1544 7145

Luxembourg • Orders 8002-2076 • Fax 8002-2073 • Technical 8002-2067

The Netherlands • Orders 0800-0229592 • Fax 0800-0229593 • Technical 0800-0229602

Norway • Orders 800-18859 • Fax 800-18817 • Technical 800-18712

Singapore • Orders 65 67775366 • Fax 65 67785177 • Technical 65 67775366

Sweden • Orders 020-790282 • Fax 020-790582 • Technical 020-798328

Switzerland • Orders 055-254-22-11 • Fax 055-254-22-13 • Technical 055-254-22-12

UK • Orders 01293 422 911 • Fax 01293 422 922 • Technical 01293 422 999

USA • Orders 800-426-8157 • Fax 800-718-2056 • Technical 800-DNA-PREP (800-362-7737)





QIAGEN
19300 Germantown Rd.
Germantown, MD 20874
Fax 800.713.2056
Ph. 800.426.8157

RECEIVED

SEP 19 12:11

STATE OF WV

Fax

To: <i>Connie Hill</i> <i>State of West Virginia</i>	Date: <i>9/19/2011</i>
Fax: <i>304-558-3970</i>	Pages: <i>5</i>
Phone: <i>304-558-0067</i>	Re: <i>Addendum #1</i> <i>RFQ # LBS12015</i>

Urgent For Review Please Comment Please Reply As Requested

*If this fax does not come through completely, please contact Stefanie Juster at (800) 426-8157 x23472 or stefanie.juster@qiagen.com. Thank you.



State of West Virginia
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Post Office Box 50130
 Charleston, WV 25305-0130

Request for Quotation

RFQ NUMBER
LBS12015

PAGE
1

ADDRESS CORRESPONDENCE TO ATTENTION OF:
**ROBERTA WAGNER
 304-558-0067**

ROBERTA WAGNER

*506084009 800-426-8157
QIAGEN INC
27220 TURNBERRY LANE STE 200

VALENCIA CA 91355-1005

SHEPHERD

**HEALTH AND HUMAN RESOURCES
 BPH - LABORATORY SERVICES**

**167-ELEVENTH AVENUE
 SOUTH CHARLESTON, WV
 25303 304-558-3530**

DATE PRINTED	TERMS OF SALE	SHIP VIA	F.O.B.	FREIGHT TERMS
09/12/2011				

BID OPENING DATE: **09/28/2011** BID OPENING TIME: **01:30PM**

LINE	QUANTITY	UOP	CAT NO	ITEM NUMBER	UNIT PRICE	AMOUNT
ADDENDUM ON: 1.						
1. QUESTIONS AND ANSWERS ARE ATTACHED.						
2. TO MOVE THE BID OPENING DATE FROM 9/15/2011 TO 9/28/2011.						
3. ADDENDUM ACKNOWLEDGEMENT IS ATTACHED. THIS DOCUMENT SHOULD BE SIGNED AND RETURNED WITH YOUR BID. FAILURE TO SIGN AND RETURN MAY RESULT IN DISQUALIFICATION OF YOUR BID.						
EXHIBIT 10						
REQUISITION NO.: LBS12015						
ADDENDUM ACKNOWLEDGEMENT						
I HEREBY ACKNOWLEDGE RECEIPT OF THE FOLLOWING CHECKED ADDENDUM(S) AND HAVE MADE THE NECESSARY REVISIONS TO MY PROPOSAL, PLANS AND/OR SPECIFICATION, ETC.						
ADDENDUM NO. S:						
NO. 1						
NO. 2						
NO. 3						
NO. 4						
NO. 5						
I UNDERSTAND THAT FAILURE TO CONFIRM THE RECEIPT OF THE ADDENDUM(S) MAY BE CAUSE FOR REJECTION OF BIDS.						

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE <i>Deby Saunders</i>	TELEPHONE 800-426-8157	DATE 9/16/2011
TITLE VP, Director Inside Sales	FEIN 95-414306	ADDRESS CHANGES TO BE NOTED ABOVE

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED "VENDOR"



State of West Virginia
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Post Office Box 50130
 Charleston, WV 25305-0130

Request for Quotation

RFQ NUMBER	PAGE
LBS12015	2

ADDRESS CORRESPONDENCE TO ATTENTION OF:

ROBERTA WAGNER
 304-558-0067

VENDOR

*506084009 800-426-8157
 QIAGEN INC
 27220 TURNBERRY LANE STE 200
 VALENCIA CA 91355-1005

SHIP TO

HEALTH AND HUMAN RESOURCES
 BPH - LABORATORY SERVICES
 167-ELEVENTH AVENUE
 SOUTH CHARLESTON, WV
 25303 304-558-3530

DATE PRINTED	TERMS OF SALE	SHIP VIA	F.O.B.	FREIGHT TERMS
09/12/2011				

BID OPENING DATE: 09/28/2011 BID OPENING TIME: 01:30PM

LINE	QUANTITY	UOP	GAT NO	ITEM NUMBER	UNIT PRICE	AMOUNT
<p>VENDOR MUST CLEARLY UNDERSTAND THAT ANY VERBAL REPRESENTATION MADE OR ASSUMED TO BE MADE DURING ANY ORAL DISCUSSION HELD BETWEEN VENDOR'S REPRESENTATIVES AND ANY STATE PERSONNEL IS NOT BINDING. ONLY THE INFORMATION ISSUED IN WRITING AND ADDED TO THE SPECIFICATIONS BY AN OFFICIAL ADDENDUM IS BINDING.</p> <p>SIGNATURE</p> <p>COMPANY</p> <p>DATE</p> <p>NOTE: THIS ADDENDUM ACKNOWLEDGEMENT SHOULD BE SUBMITTED WITH THE BID.</p> <p>REV. 09/21/2009</p> <p>END OF ADDENDUM NO. 1</p>						

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE	TELEPHONE	DATE
<i>Delby Jansen</i>	800-426-8157	9/16/2011
TITLE	FEIN	ADDRESS CHANGES TO BE NOTED ABOVE
VP, Director Inside Sales	95-4141306	

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED 'VENDOR'



State of West Virginia
 Department of Administration
 Purchasing Division
 2019 Washington Street East
 Post Office Box 50130
 Charleston, WV 25305-0130

Request for Quotation

RFQ NUMBER
LBS12015

PAGE
3

ADDRESS CORRESPONDENCE TO ATTENTION OF:
**ROBERTA WAGNER
 304-558-0067**

VENDOR

*506084009 800-426-8157
QIAGEN INC
27220 TURNBERRY LANE STE 200
VALENCIA CA 91355-1005

SHIP TO

**HEALTH AND HUMAN RESOURCES
 BPH - LABORATORY SERVICES**
**167-ELEVENTH AVENUE
 SOUTH CHARLESTON, WV
 25303 304-558-3530**

DATE PRINTED	TERMS OF SALE	SHIP VIA	F.O.B.	FREIGHT TERMS
09/12/2011				

BID OPENING DATE: **09/28/2011** BID OPENING TIME: **01:30PM**

LINE	QUANTITY	UOP	CAT NO.	ITEM NUMBER	UNIT PRICE	AMOUNT
0001	1	JB		193-36		
				AUTOMATED NUCLEIC ACID PURIFICATION SYSTEM		
***** THIS IS THE END OF RFQ LBS12015 ***** TOTAL:						

SEE REVERSE SIDE FOR TERMS AND CONDITIONS

SIGNATURE <i>Roberta Wagner</i>	TELEPHONE 800-426-8157	DATE 9/16/2011
TITLE VP, Director Inside Sales	FEIN 95-4141306	ADDRESS CHANGES TO BE NOTED ABOVE

WHEN RESPONDING TO RFQ, INSERT NAME AND ADDRESS IN SPACE ABOVE LABELED "VENDOR"

WV-36 (Rev. 01/01/07)

STATE OF WEST VIRGINIA
PURCHASE CONTINUATION SHEET

Page _____ of _____ Pages

Requisition / P.O. No.:
 LBS12015

File:

Acct. No.:

8802-2012-2958-096-072-19465

Spending Unit:

DHHRVOLS

Vendor: _____ P.O. Date: _____

Item No.	Quantity	Description	Unit Price	Amount
		<p>VENDOR QUESTION #1:</p> <p>Could you please explain what is meant by FDA approved?</p> <p>RESPONSE:</p> <p>The reference to the FDA, is in regards to a protocol that is used for a particular instrument that has been approved by the FDA.</p>		
		<p>VENDOR QUESTION #2:</p> <p>Since this appears to be very similar to RFQ LBS12058- would I be able to actually see why this original RFQ was canceled? Are those bids visual to the public?</p> <p>RESPONSE:</p> <p>Yes, the bids can be viewed or copies requested through the archive area.</p>		