



# West Virginia Purchasing Division

2019 Washington Street, East  
Charleston, WV 25305  
Telephone: 304-558-2306  
General Fax: 304-558-6026  
Bid Fax: 304-558-3970

The following documentation is an electronically-submitted vendor response to an advertised solicitation from the *West Virginia Purchasing Bulletin* within the Vendor Self-Service portal at [wvOASIS.gov](http://wvOASIS.gov). As part of the State of West Virginia's procurement process, and to maintain the transparency of the bid-opening process, this documentation submitted online is publicly posted by the West Virginia Purchasing Division at [WVPurchasing.gov](http://WVPurchasing.gov) with any other vendor responses to this solicitation submitted to the Purchasing Division in hard copy format.

## Header 5

List View

[General Information](#) [Contact](#) [Default Values](#) [Discount](#) [Document Information](#) [Clarification Request](#)

Procurement Folder: 1841869

SO Doc Code: CRFQ

Procurement Type: Central Purchase Order

SO Dept: 1400

Vendor ID: VS0000011637



Legal Name: STERILELINK INC

SO Doc ID: AGR2600000024

Alias/DBA:

Published Date: 1/23/26

Total Bid: \$188,670.00

Close Date: 2/3/26

Response Date: 02/03/2026




Close Time: 13:30

Response Time: 10:41

Status: Closed

Responded By User ID: Sterilelink



Total of Header Attachments: 5

First Name: Jason

Total of All Attachments: 5

Last Name: Harrington

Email: info@sterilelink.com

Phone: 336-254-2266



Department of Administration  
Purchasing Division  
2019 Washington Street East  
Post Office Box 50130  
Charleston, WV 25305-0130

**State of West Virginia  
Solicitation Response**

**Proc Folder:** 1841869

**Solicitation Description:** READ - Laboratory Steam Sterilizers

**Proc Type:** Central Purchase Order

Solicitation Closes	Solicitation Response	Version
2026-02-03 13:30	SR 1400 ESR0202260000004432	1

**VENDOR**

VS0000011637  
STERILELINK INC

**Solicitation Number:** CRFQ 1400 AGR2600000024

**Total Bid:** 188670

**Response Date:** 2026-02-03

**Response Time:** 10:41:09

**Comments:**

**FOR INFORMATION CONTACT THE BUYER**

Larry D McDonnell  
304-558-2063  
larry.d.mcdonnell@wv.gov

Vendor  
Signature X

FEIN#

DATE

All offers subject to all terms and conditions contained in this solicitation

Line	Comm Ln Desc	Qty	Unit Issue	Unit Price	Ln Total Or Contract Amount
1	Discard Autoclave Laboratory Steam Sterilizer section 3.1.1	2.00000	EA	60051.000000	120102.00

Comm Code	Manufacturer	Specification	Model #
42281508			

**Commodity Line Comments:** Discard Autoclave Laboratory Steam Sterilizer specification section 3.1.1  
Tuttnauer™ Model 5596-ECP-V Pre-Vac Steam Sterilizer

**Extended Description:**

Discard Autoclave Laboratory Steam Sterilizer specification section 3.1.1  
See attached specification and associated documentation for further details.

Line	Comm Ln Desc	Qty	Unit Issue	Unit Price	Ln Total Or Contract Amount
2	Media Autoclave Laboratory Steam Sterilizer section 3.1.2	1.00000	EA	53268.000000	53268.00

Comm Code	Manufacturer	Specification	Model #
42281508			

**Commodity Line Comments:** Media Autoclave Laboratory Steam Sterilizer section 3.1.2  
Tuttnauer™ Model 4472-ECP-V Pre-Vac Steam Sterilizer

**Extended Description:**

Media Autoclave Laboratory Steam Sterilizer specification section 3.1.2  
See attached specification and associated documentation for further details.

Line	Comm Ln Desc	Qty	Unit Issue	Unit Price	Ln Total Or Contract Amount
3	Warranty/Preventative Maintenance Service section 3.1.3	1.00000	EA	0.000000	0.00

Comm Code	Manufacturer	Specification	Model #
42281508			

**Commodity Line Comments:** NO CHARGE

**Extended Description:**

Warranty/Preventative Maintenance Service specification section 3.1.3  
See attached specification and associated documentation for further details.

Line	Comm Ln Desc	Qty	Unit Issue	Unit Price	Ln Total Or Contract Amount
4	Installation sections 3.1.1.13 and 3.1.2.13	1.00000	EA	14400.000000	14400.00

Comm Code	Manufacturer	Specification	Model #
42281508			

**Commodity Line Comments:** Sterilelink Installation According to Specs

**Extended Description:**

Installation specification sections 3.1.1.13 and 3.1.2.13  
See attached specification and associated documentation for further details.

Line	Comm Ln Desc	Qty	Unit Issue	Unit Price	Ln Total Or Contract Amount
5	Onsite Training sections 3.1.1.13 and 3.1.2.13	1.00000	EA	900.000000	900.00

Comm Code	Manufacturer	Specification	Model #
42281508			


**Commodity Line Comments:**

**Extended Description:**


Onsite Training specifications sections 3.1.1.13 and 3.1.2.13

See attached specification and associated documentation for further details.


### Side View

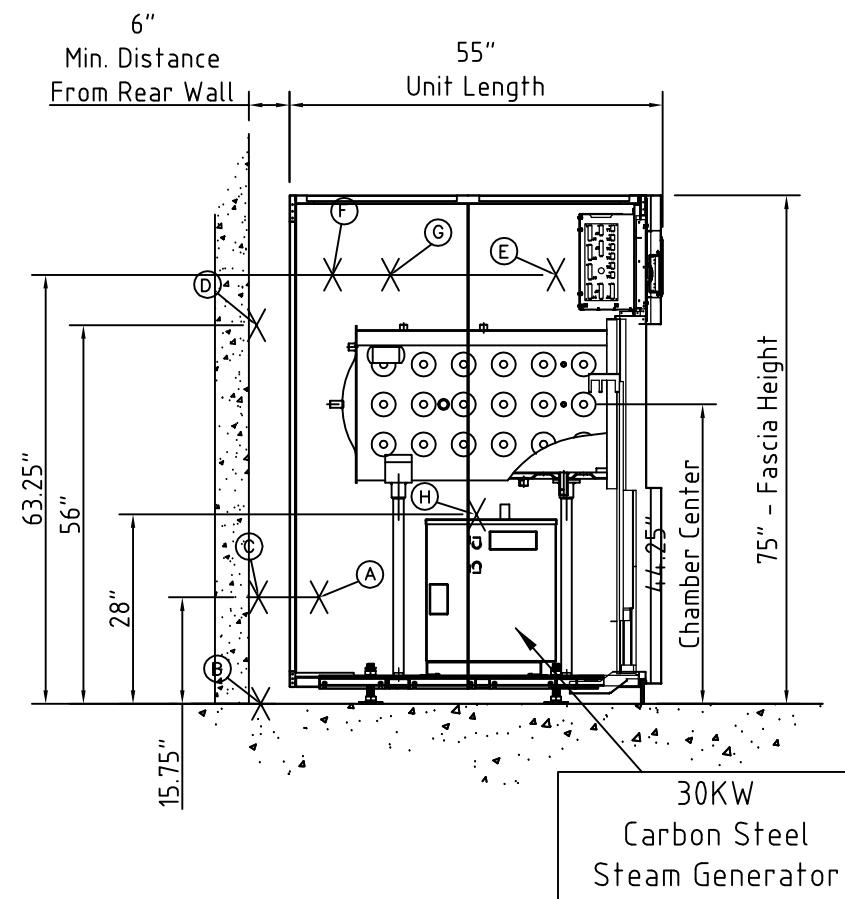

### Front View

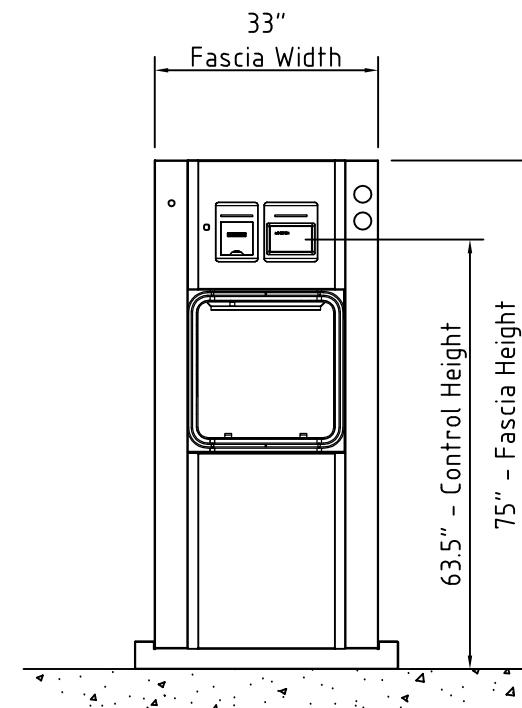

### Top View

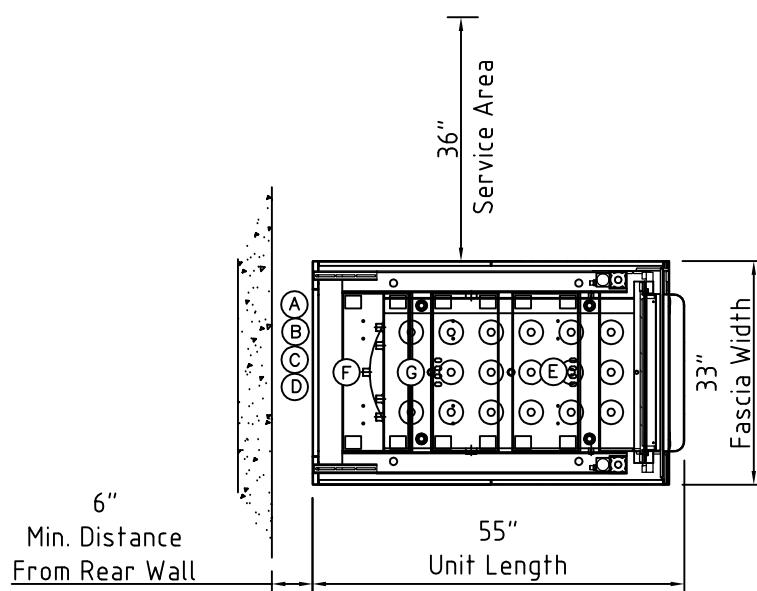

FOR REFERENCE ONLY - NOT FOR CONSTRUCTION!

#### PLEASE NOTE:

1. Minimum 36" wide doorways (34.5" clear opening) required for autoclave transport, with free and clear path.
2. 3-phase electrical supply must be installed by others, located within 5' of rear of sterilizer and connected to an appropriate electrical disconnect, as per local codes and regulations.
3. Autoclave can be provided with either left or right side piping/service access. Right side piping/service access currently shown.

This document is PROPRIETARY to Tuttnauer Co. Ltd. and it and its contents may not be disseminated to anyone outside your organization or anyone within your organization who does not have a need to know its contents

#### REVISIONS

REV.	DESCRIPTION	DATE	APPROVED

#### MODEL 5596-ECP-V

INTERIOR CHAMBER DIMENSION: 20"x20"x38"

#### UTILITIES REQUIREMENTS

A - RO Water Supply for Carbon Steel Electric Steam Generator - 1/2" NPT with Ball Valve, 1 GPM Peak, 5 Gallons Per Cycle Average (See GENERAL UTILITY GUIDELINES for Recommended Water Quality)

B - System Drain - ( Outlet 1" NPT ) - 2" O.D.T. Located by others. Floor Sink Recommended.

C - Cold Water Supply - 3/4", <70 Degrees F, 45 PSI Dynamic Minimum, 8 GPM Peak.

D - Compressed Air - 90 PSI Minimum, 3.5 SCFM, 3/8" NPT with Ball Valve

E - Electric Power Supply:

BACSOFT CONTROL - 120V, 1 phase, 20 AMP. (Dedicated Line)

CHOICE OF: CARBON STEEL ELECTRIC STEAM GENERATOR - 30 KW, 208V, 3 phase, 84 AMP. (Draw)  
OR CARBON STEEL ELECTRIC STEAM GENERATOR - 30 KW, 480V, 3 phase, 37 AMP. (Draw)

F - Chamber Relief Exhaust Valve - 3/4"

G - Jacket Relief Exhaust Valve - 3/4"

H - Carbon Steel Steam Generator Relief Exhaust Valve - 1"

#### HEAT LOSS

- With door open - 6070 Btu / hr at 68°F

#### WEIGHT


- Autoclave - 1700 lb Operating - 2262 lb

#### GENERAL NOTES


1. Utilities shown are required at sterilizer within 36" terminating with a shutoff valve.
2. The sterilizer is not supplied with a back flow preventer and, when required by local codes, to be provided and installed by others.
3. Floor Sink Recommended at the side of sterilizer.
4. Safety Relief valves will be piped to floor by installer.
5. If local code requires that relief valves be piped with an alternate method, to be responsibility of others.
6. All wiring up to the sterilizer disconnects to be installed by others.
7. All disconnect switches to be installed by others.
8. Pipe sizes shown indicate terminal outlets only, service lines must supply the specified pressure and flow rates.
9. Clearances shown are minimal for installing and servicing the equipment.
10. All locations of utilities and clearances will be shown on architectural drawings.
11. Drain location can be placed to the side if no space is available behind sterilizer.
12. Softened water systems may be used only when properly maintained. Please note that malfunctioning water softeners can cause damage to the generator and will void the warranty.
13. Some states require that an emergency stop be provided external to the sterilizer. If an external emergency stop is required by local codes, to be provided and installed by others.
14. See GENERAL UTILITY GUIDELINES.

#### CUSTOMER: West Virginia Dept of Agriculture

	Description:	Tolerance: .N.A		
		5596-ECP-V, 20"x20"x38"	Job No.:	Scale:
	Material:	Design:	Drawing: Sara D.	Quant./Unit: 1
ISO A2	Rev.No:	00	Preparation By: Sara D. 01-26-2026	Approved By:

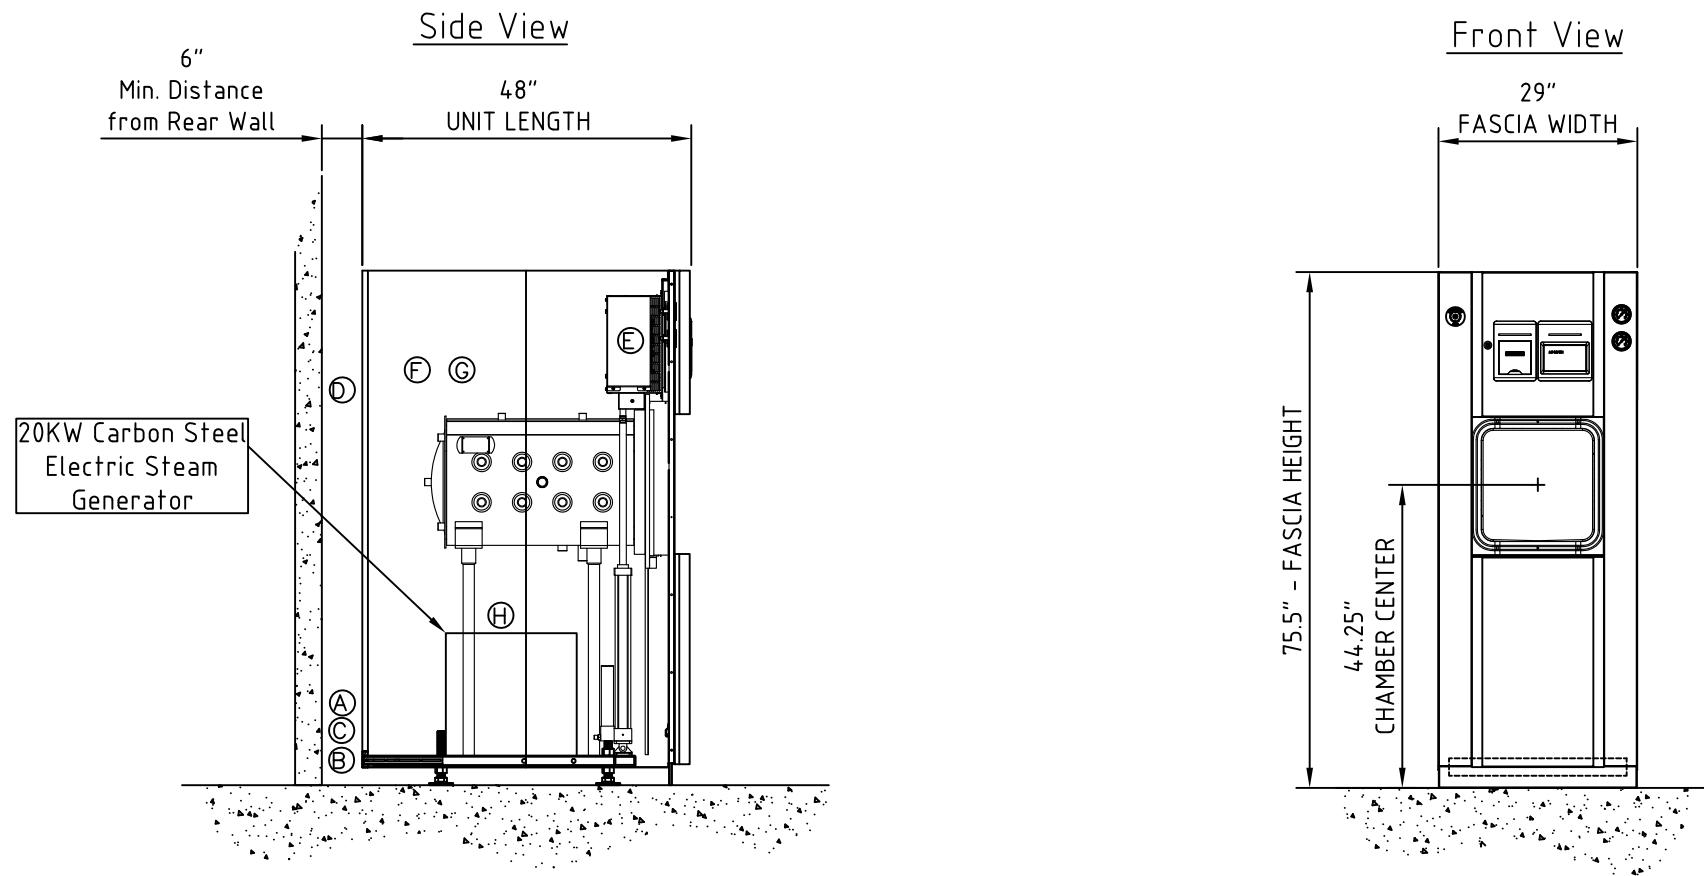

### Top View

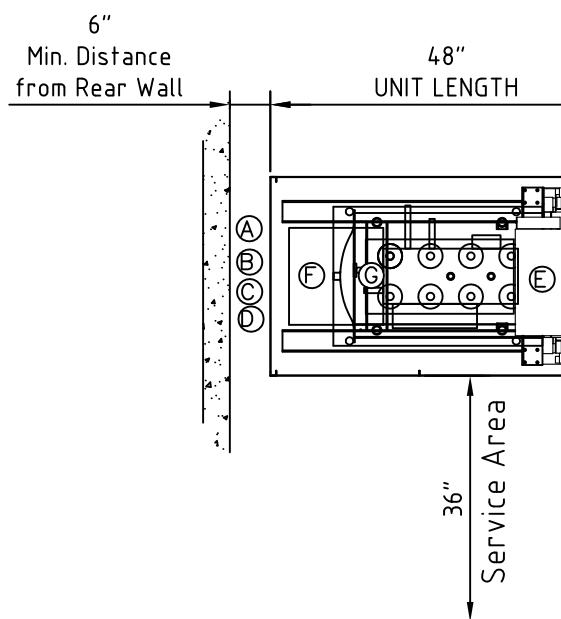

FOR REFERENCE ONLY - NOT FOR CONSTRUCTION!

## PLEASE NOTE:

1. Minimum 36" wide doorways (34.5" clear pathway) required for autoclave transport, with free and clear path.
2. 3-phase electrical supply must be installed by others, located within 5' of rear of sterilizer and connected to an appropriate electrical disconnect, as per local codes and regulations.
3. Autoclave can be provide with either left or right side piping/service access. Left side piping/service access currently shown.

This document is PROPRIETARY to Tuttnauer Co. Ltd. and it and its contents may not be disseminated to anyone outside your organization or anyone within your organization who does not have a need to know its contents

## REVISIONS

REV.	DESCRIPTION	DATE	APPROVED

MODEL 4472-ECP-V

INTERIOR CHAMBER DIMENSION: 16" x 16" x 28"

## UTILITIES REQUIREMENTS

A - RO Water Supply for Carbon Steel Electric Steam Generator -  
1/2" NPT with Ball Valve, 1 GPM Peak, 5 Gallons Per Cycle Average  
(See GENERAL UTILITY GUIDELINES for Recommended Water Quality)

B - System Drain - ( Outlet 1" NPT ) - 2" O.D.T. Located by others. Floor Sink Recommended.

C - Cold Water Supply - 3/4" NPT with Ball Valve, <70 Degrees F, 45 PSI Dynamic Minimum, 8 GPM Peak

D - Compressed Air - 90 PSI Minimum, 3.5 SCFM, 3/8" NPT with Ball Valve

E - Electric Power Supply for:  
BACSOFT CONTROL - 120V, 1 phase, 20 AMP. (Dedicated Line)  
CHOICE OF:    CARBON STEEL ELECTRIC STEAM GENERATOR - 20 KW, 208V, 3 phase, 56 AMP. (Draw)  
OR            CARBON STEEL ELECTRIC STEAM GENERATOR - 20 KW, 480V, 3 phase, 25 AMP. (Draw)

#### E - Chamber Relief Exhaust Valve - 3/4"

1 - CHAMBER RELIEF EXHAUST VALVE - 3/4"

### G - Jacket Re

## H - Carbon Steel Steam Generator Relief B

## HEAT LOSS

HEAT LOSS

### WEIGHT


WEIGHT - Autoclave - 1400 lb Operating - 1660 lb

#### GENERAL NOTES

**GENERAL NOTES**

1. Utilities shown are required at sterilizer within 36" terminating with a shutoff valve.
2. The sterilizer is not supplied with a back flow preventer and, when required by local codes, to be provided and installed by others.
3. Floor Sink Recommended at the side of sterilizer.
4. Safety Relief valves will be piped to floor by installer.
5. If local code requires that relief valves be piped with an alternate method, to be responsibility of others.
6. All wiring up to the sterilizer disconnects to be installed by others.
7. All disconnect switches to be installed by others.
8. Pipe sizes shown indicate terminal outlets only, service lines must supply the specified pressure and flow rates.
9. Clearances shown are minimal for installing and servicing the equipment.
10. All locations of utilities and clearances will be shown on architectural drawings.
11. Drain location can be placed to the side if no space is available behind sterilizer.
12. Softened water systems may be used only when properly maintained. Please note that malfunctioning water softeners can cause damage to the generator and will void the w...
13. Some states require that an emergency stop be provided external to the sterilizer. If an external emergency stop is required by local codes, to be provided and installed by oth...
14. See GENERAL UTILITY GUIDELINES.

Customer: West Virginia Dept of Agriculture

Customer: West Virginia Dept of Agriculture					Tolerance: .N.A	
	Description: 4472-ECP-V, 16"x16"x28"		4472-ECP-V	Job No.:	Scale:	Drawing No.:
	Material:	Design:	Drawing: Sara D. 1-26-2026	Quant./Unit: 1	Quant./Job:	
		Rev.No: 00	Preparation By: Sara D. 1-26-2026	Approved By:	Q.C.:	
 <span>ISO A2</span>						

**Sterilelink, Inc.**  
PO Box 16125  
Greensboro, NC 27416  
USA  
+13362542266  
[info@sterilelink.com](mailto:info@sterilelink.com)  
[www.sterilelink.com](http://www.sterilelink.com)



ADDRESS	SHIP TO
West Virginia Dept Agriculture 313 Gus R Douglas Lane Charleston, WV 25312	REGULATORY PROTECTION DIVISION 313 Gus R Douglas Lane Charleston, WV 25312

**Quote 14478**

**DATE 02/03/2026**

**EXPIRATION DATE 04/30/2026**

**SALES REP**  
Jason Harrington

**REPORT**  
CRFQ AGR26\*24

DATE	ACTIVITY	QTY	RATE	AMOUNT
------	----------	-----	------	--------

Sterilelink is ISO 9001:2015 Certified Registration Number 24-R1646  
A 3% processing fee will be added for credit card payments.  
All Invoices are due and payable upon receipt, and past due 30 days after date.

DATE	ACTIVITY	QTY	RATE	AMOUNT
	<p><b>Sterilizer</b>  Discard Autoclave Laboratory Steam Sterilizer  specification section 3.1.1</p> <p>TuttnauerTM Model 5596-ECP-V Pre-Vac Steam Sterilizer  Internal Chamber Dimensions: 20W x 20H x 38D  Door Configuration: Single, Automatic Vertical Sliding Door  Steam Supply: Integral 30KW Carbon Steel Electric Steam  Generator with Automatic Blow Down (3-Phase Power Required, 208V or 480V)  Mounting: Free-Standing with Stainless Steel Cabinet  Controls: BacSoft Microprocessor with 7" Color Touch Screen  Printer: Alphanumeric, Thermal  Cycles: Gravity, Liquid, Pre-Vac  Test Cycles: Vacuum Leak Test, Bowie Dick Test  Piping: Stainless Steel Threaded  Components: Brass and Stainless Steel (Non-Proprietary)  Valves: Air-Operated Valves  Air Source: House Supplied (90 PSI Minimum Required)  Vacuum System: Water Ejector  Condensate Cooler: Effluent cooled to below 140 degrees  Chamber: 316L Stainless Steel  Jacket: 304L Stainless Steel  Loading Equipment: Rack and Two Shelves  1-Year Parts and Labor Warranty (Labor provided by Dealer)  15-Year Pressure Vessel Warranty</p>	2	60,051.00	120,102.00T

Sterilelink is ISO 9001:2015 Certified Registration Number 24-R1646

A 3% processing fee will be added for credit card payments.

All Invoices are due and payable upon receipt, and past due 30 days after date.

DATE	ACTIVITY	QTY	RATE	AMOUNT
	<b>Services</b> Media Autoclave Laboratory Steam Sterilizer section 3.1.2 TuttnauerTM Model 4472-ECP-V Pre-Vac Steam Sterilizer Internal Chamber Dimensions: 16W x 16H x 28D Door Configuration: Single, Automatic Vertical Sliding Door Steam Supply: Integral 20KW Carbon Steel Electric Steam Generator with Automatic Blow Down (3-Phase Power Required, 208V or 480V) Mounting: Free-Standing with Stainless Steel Cabinet Controls: BacSoft Microprocessor with 7" Color Touch Screen Printer: Alphanumeric, Thermal Cycles: Gravity, Liquid, Pre-Vac Test Cycles: Vacuum Leak Test, Bowie Dick Test Piping: Stainless Steel Threaded Components: Brass and Stainless Steel (Non- Proprietary) Valves: Air-Operated Valves Air Source: House Supplied (90 PSI Minimum Required) Vacuum System: Water Ejector Condensate Cooler: Effluent cooled to below 140 degrees Chamber: 316L Stainless Steel Jacket: 304L Stainless Steel Loading Equipment: Rack and Two Shelves 1-Year Parts and Labor Warranty (Labor provided by Dealer) 15-Year Pressure Vessel Warranty	1	53,268.00	53,268.00T
	<b>Standard Installation</b> Installation sections 3.1.1.13 and 3.1.2.13	3	4,800.00	14,400.00T
	<b>Warranty</b> Warranty/Preventative Maintenance Service section 3.1.3 Manufacturer Warranty included for 1 year service provided by Sterilelink	1	0.00	0.00T
	<b>Service</b> Onsite Training sections 3.1.1.13 and 3.1.2.13 Training provided by Sterilelink	1	900.00	900.00T

Sterilelink is ISO 9001:2015 Certified Registration Number 24-R1646

A 3% processing fee will be added for credit card payments.

All Invoices are due and payable upon receipt, and past due 30 days after date.

DATE	ACTIVITY	QTY	RATE	AMOUNT
	<b>Terms &amp; Conditions (365)</b>	1	0.00	0.00T
	1. No State or Federal Taxes included.			
	2. Warranty: Parts and associated labor: 365 days from date of installation by Sterilelink Representative or 3 months from acceptance of delivery to facility or storage.			
	3. Delivery 90-120 days from receipt of approval drawings.			
	4. Pricing firm until expiration date of quote.			
	5. Start-up and staff training by Dealer Representative.			
	6. Payment terms: 50% with order, 30% on delivery, balance due 30 days following installation.			
	7. Purchase order and/or payment to be issued directly to Sterilelink, Inc.			
	8. Cancellation: This order cannot be canceled or modified, or releases hereunder held up by Buyer after order is in process, except with the Company consent and subject to conditions then to be agreed upon which shall include protection of the Company against all loss including but not limited to all cost incurred at time of cancellation notice by buyer, and in no event shall cancellation charge be less than 20% of price of order.			
	9. The title and ownership of said materials and equipment shall remain vested in the Seller until the purchase price has been paid in full. Purchaser shall not permit any lien or encumbrance or security interest adverse to Seller's title to be placed on the items being sold hereunder.			
	10. Due to current shipping issues changes in freight fluctuate daily all freight charges will be confirmed at time of order but are subject to change due to circumstances beyond our control			
		SUBTOTAL		188,670.00
		TAX (0%)		0.00
		TOTAL		<b>\$188,670.00</b>

Accepted By

Accepted Date

Sterilelink is ISO 9001:2015 Certified Registration Number 24-R1646

A 3% processing fee will be added for credit card payments.

All Invoices are due and payable upon receipt, and past due 30 days after date.

**DESIGNATED CONTACT:** Vendor appoints the individual identified in this Section as the Contract Administrator and the initial point of contact for matters relating to this Contract.

JASON HARRINGTON

(Printed Name and Title) \_\_\_\_\_

(Address) \_\_\_\_\_ 500 SUNSET AVENUE ASHEBORO NC 27203

(Phone Number) / (Fax Number) \_\_\_\_\_ 335-254-2266

(email address) \_\_\_\_\_ info@sterilelink.com

**CERTIFICATION AND SIGNATURE:** By signing below, or submitting documentation through wvOASIS, I certify that: I have reviewed this Solicitation/Contract in its entirety; that I understand the requirements, terms and conditions, and other information contained herein; that this bid, offer or proposal constitutes an offer to the State that cannot be unilaterally withdrawn; that the product or service proposed meets the mandatory requirements contained in the Solicitation/Contract for that product or service, unless otherwise stated herein; that the Vendor accepts the terms and conditions contained in the Solicitation, unless otherwise stated herein; that I am submitting this bid, offer or proposal for review and consideration; that this bid or offer was made without prior understanding, agreement, or connection with any entity submitting a bid or offer for the same material, supplies, equipment or services; that this bid or offer is in all respects fair and without collusion or fraud; that this Contract is accepted or entered into without any prior understanding, agreement, or connection to any other entity that could be considered a violation of law; that I am authorized by the Vendor to execute and submit this bid, offer, or proposal, or any documents related thereto on Vendor's behalf; that I am authorized to bind the vendor in a contractual relationship; and that to the best of my knowledge, the vendor has properly registered with any State agency that may require registration.

*By signing below, I further certify that I understand this Contract is subject to the provisions of West Virginia Code § 5A-3-62, which automatically voids certain contract clauses that violate State law; and that pursuant to W. Va. Code 5A-3-63, the entity entering into this contract is prohibited from engaging in a boycott against Israel.*

Sterilelink, Inc

(Company) \_\_\_\_\_

*Jason Harrington*

(Signature of Authorized Representative) \_\_\_\_\_  
Jason Harrington Vice President

(Printed Name and Title of Authorized Representative) (Date)  
336-254-2266

(Phone Number) (Fax Number)  
info@sterilelink.com

(Email Address) \_\_\_\_\_

**ADDENDUM ACKNOWLEDGEMENT FORM**  
**SOLICITATION NO.: CRFQ AGR26\*24**

**Instructions:** Please acknowledge receipt of all addenda issued with this solicitation by completing this addendum acknowledgment form. Check the box next to each addendum received and sign below. Failure to acknowledge addenda may result in bid disqualification.

**Acknowledgment:** I hereby acknowledge receipt of the following addenda and have made the necessary revisions to my proposal, plans and/or specification, etc.

**Addendum Numbers Received:**

(Check the box next to each addendum received)

<input checked="" type="checkbox"/> Addendum No. 1	<input type="checkbox"/> Addendum No. 6
<input checked="" type="checkbox"/> Addendum No. 2	<input type="checkbox"/> Addendum No. 7
<input type="checkbox"/> Addendum No. 3	<input type="checkbox"/> Addendum No. 8
<input type="checkbox"/> Addendum No. 4	<input type="checkbox"/> Addendum No. 9
<input type="checkbox"/> Addendum No. 5	<input type="checkbox"/> Addendum No. 10

I understand that failure to confirm the receipt of addenda may be cause for rejection of this bid. I further understand that any verbal representation made or assumed to be made during any oral discussion held between Vendor's representatives and any state personnel is not binding. Only the information issued in writing and added to the specifications by an official addendum is binding.

Sterilelink Inc.

---

Company

---

*Jason Harrington*

---

Authorized Signature

02/03/2026

---

Date

NOTE: This addendum acknowledgement should be submitted with the bid to expedite document processing.



Department of Administration  
Purchasing Division  
2019 Washington Street East  
Post Office Box 50130  
Charleston, WV 25305-0130

**State of West Virginia  
Centralized Request for Quote  
Laboratory**

<b>Proc Folder:</b> 1841869	<b>Reason for Modification:</b>		
<b>Doc Description:</b> READ - Laboratory Steam Sterilizers	Addendum No. 02		
<b>Proc Type:</b> Central Purchase Order			
<b>Date Issued</b>	<b>Solicitation Closes</b>	<b>Solicitation No</b>	<b>Version</b>
2026-01-23	2026-02-03 13:30	CRFQ 1400 AGR2600000024	3

#### **BID RECEIVING LOCATION**

BID CLERK  
DEPARTMENT OF ADMINISTRATION  
PURCHASING DIVISION  
2019 WASHINGTON ST E  
CHARLESTON WV 25305  
US

#### **VENDOR**

##### **Vendor Customer Code:**

**Vendor Name :** Sterilelink Inc.

**Address :** 500

**Street :** Sunset Ave

**City :** Asheboro

**State :** NC

**Country :** USA

**Zip :** 27203

**Principal Contact :** Jason Harrington

**Vendor Contact Phone:** 336-254-2266

**Extension:**

#### **FOR INFORMATION CONTACT THE BUYER**

Larry D McDonnell  
304-558-2063  
larry.d.mcdonnell@wv.gov

*Jason Harrington*

**Vendor  
Signature X**

**FEIN#** 14-1924248

**DATE** 02/02/2026

**All offers subject to all terms and conditions contained in this solicitation**

**ADDITIONAL INFORMATION**

Addendum No. 02

To post answers to vendor questions.

Bid opening date and time remains 02/03/2026 at 1:30PM EST/EDT

No other changes

INVOICE TO	SHIP TO
AGRICULTURE DEPARTMENT OF ADMINISTRATIVE SERVICES  1900 KANAWHA BLVD E  CHARLESTON US	AGRICULTURE DEPARTMENT OF REGULATORY PROTECTION DIVISION  313 GUS R DOUGLAS LN, BLDG 11  CHARLESTON WV US

Line	Comm Ln Desc	Qty	Unit Issue	Unit Price	Total Price
1	Discard Autoclave Laboratory Steam Sterilizer section 3.1.1	2.00000	EA		

Comm Code	Manufacturer	Specification	Model #
42281508			

**Extended Description:**

Discard Autoclave Laboratory Steam Sterilizer specification section 3.1.1

See attached specification and associated documentation for further details.

INVOICE TO	SHIP TO
AGRICULTURE DEPARTMENT OF ADMINISTRATIVE SERVICES  1900 KANAWHA BLVD E  CHARLESTON US	AGRICULTURE DEPARTMENT OF REGULATORY PROTECTION DIVISION  313 GUS R DOUGLAS LN, BLDG 11  CHARLESTON WV US

Line	Comm Ln Desc	Qty	Unit Issue	Unit Price	Total Price
2	Media Autoclave Laboratory Steam Sterilizer section 3.1.2	1.00000	EA		

Comm Code	Manufacturer	Specification	Model #
42281508			

**Extended Description:**

Media Autoclave Laboratory Steam Sterilizer specification section 3.1.2

See attached specification and associated documentation for further details.

INVOICE TO	SHIP TO
AGRICULTURE DEPARTMENT OF ADMINISTRATIVE SERVICES  1900 KANAWHA BLVD E  CHARLESTON US	AGRICULTURE DEPARTMENT OF REGULATORY PROTECTION DIVISION  313 GUS R DOUGLAS LN, BLDG 11  CHARLESTON WV US

Line	Comm Ln Desc	Qty	Unit Issue	Unit Price	Total Price
3	Warranty/Preventative Maintenance Service section 3.1.3	1.00000	EA		

Comm Code	Manufacturer	Specification	Model #
42281508			

**Extended Description:**

Warranty/Preventative Maintenance Service specification section 3.1.3

See attached specification and associated documentation for further details.

INVOICE TO		SHIP TO		
AGRICULTURE DEPARTMENT OF ADMINISTRATIVE SERVICES		AGRICULTURE DEPARTMENT OF REGULATORY PROTECTION DIVISION		
1900 KANAWHA BLVD E CHARLESTON US		313 GUS R DOUGLAS LN, BLDG 11 CHARLESTON US		
Line	Comm Ln Desc	Qty	Unit Issue	Unit Price
4	Installation sections 3.1.1.13 and 3.1.2.13	1.00000	EA	

Comm Code	Manufacturer	Specification	Model #
42281508			

**Extended Description:**

Installation specification sections 3.1.1.13 and 3.1.2.13

See attached specification and associated documentation for further details.

INVOICE TO		SHIP TO		
AGRICULTURE DEPARTMENT OF ADMINISTRATIVE SERVICES		AGRICULTURE DEPARTMENT OF REGULATORY PROTECTION DIVISION		
1900 KANAWHA BLVD E CHARLESTON US		313 GUS R DOUGLAS LN, BLDG 11 CHARLESTON US		
Line	Comm Ln Desc	Qty	Unit Issue	Unit Price
5	Onsite Training sections 3.1.1.13 and 3.1.2.13	1.00000	EA	

Comm Code	Manufacturer	Specification	Model #
42281508			

**Extended Description:**

Onsite Training specifications sections 3.1.1.13 and 3.1.2.13

See attached specification and associated documentation for further details.

SCHEDULE OF EVENTS		
Line	Event	Event Date
1	Vendor questions due by 2:00PM EST/EDT	2026-01-16

	Document Phase	Document Description	Page
			5
AGR2600000024	Final	READ - Laboratory Steam Sterilizers	

#### **ADDITIONAL TERMS AND CONDITIONS**

See attached document(s) for additional Terms and Conditions